

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
 Data File : VU046839.D
 Acq On : 26 Jan 2022 12:32
 Operator : SY/MD
 Sample : N1260-02 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFX4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046839.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.362	3	7	17	rVB2	18231	19361	4.90%	0.617%
2	1.604	73	82	96	rVB	47551	59778	15.12%	1.906%
3	1.919	172	180	197	rBV	35470	48277	12.21%	1.540%
4	2.160	250	255	265	rVB4	3115	4656	1.18%	0.148%
5	2.575	373	384	399	rBV	72282	115633	29.25%	3.688%
6	3.054	524	533	543	rVB2	3889	6725	1.70%	0.214%
7	4.658	1015	1032	1069	rBV2	36107	153515	38.84%	4.896%
8	5.070	1143	1160	1186	rBV2	64793	146926	37.17%	4.686%
9	5.729	1343	1365	1387	rBV2	122259	327434	82.83%	10.442%
10	6.253	1514	1528	1546	rBV	148745	281251	71.15%	8.969%
11	6.697	1652	1666	1684	rBV2	79031	152088	38.48%	4.850%
12	7.568	1926	1937	1958	rVB	34997	61043	15.44%	1.947%
13	7.902	2024	2041	2055	rBV	139822	244933	61.96%	7.811%
14	8.182	2118	2128	2147	rBV3	22971	38109	9.64%	1.215%
15	8.639	2257	2270	2297	rBV	206970	375575	95.01%	11.977%
16	8.915	2346	2356	2368	rBV3	5064	7921	2.00%	0.253%
17	9.420	2500	2513	2546	rBV	236291	395288	100.00%	12.606%
18	10.758	2917	2929	2946	rBV	70161	112978	28.58%	3.603%
19	11.812	3244	3257	3273	rBV	233051	364127	92.12%	11.612%
20	12.195	3363	3376	3395	rVB	133956	220074	55.67%	7.018%




Sum of corrected areas: 3135692

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046839.D
Acq On : 26 Jan 2022 12:32
Operator : SY/MD
Sample : N1260-02 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

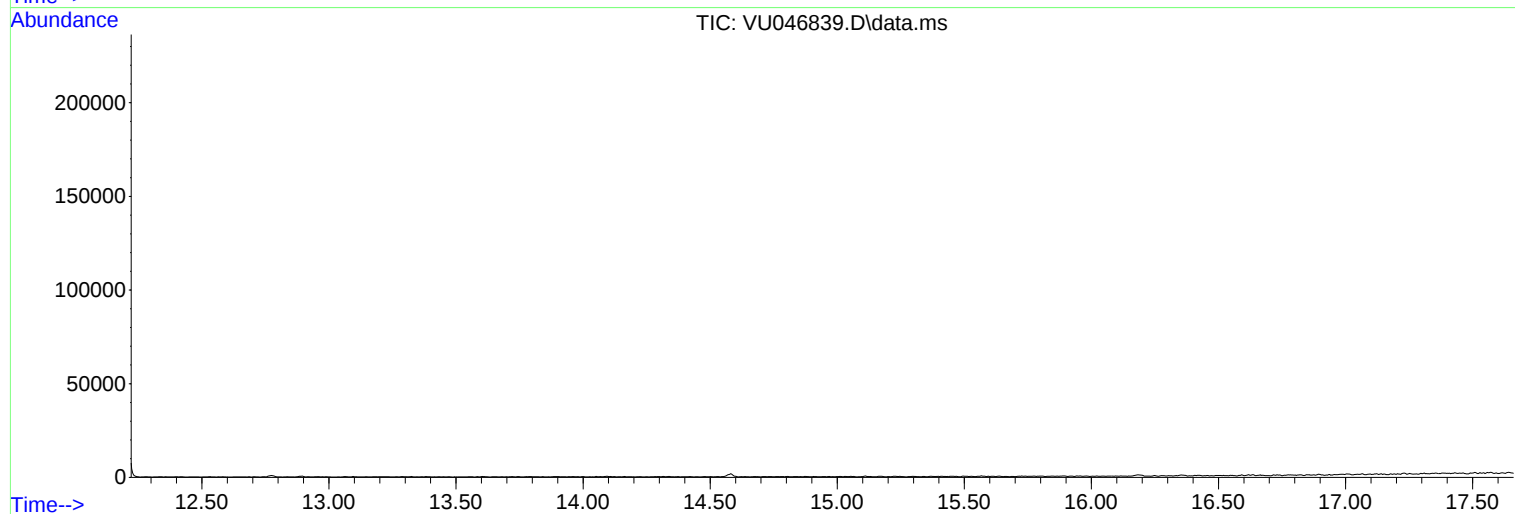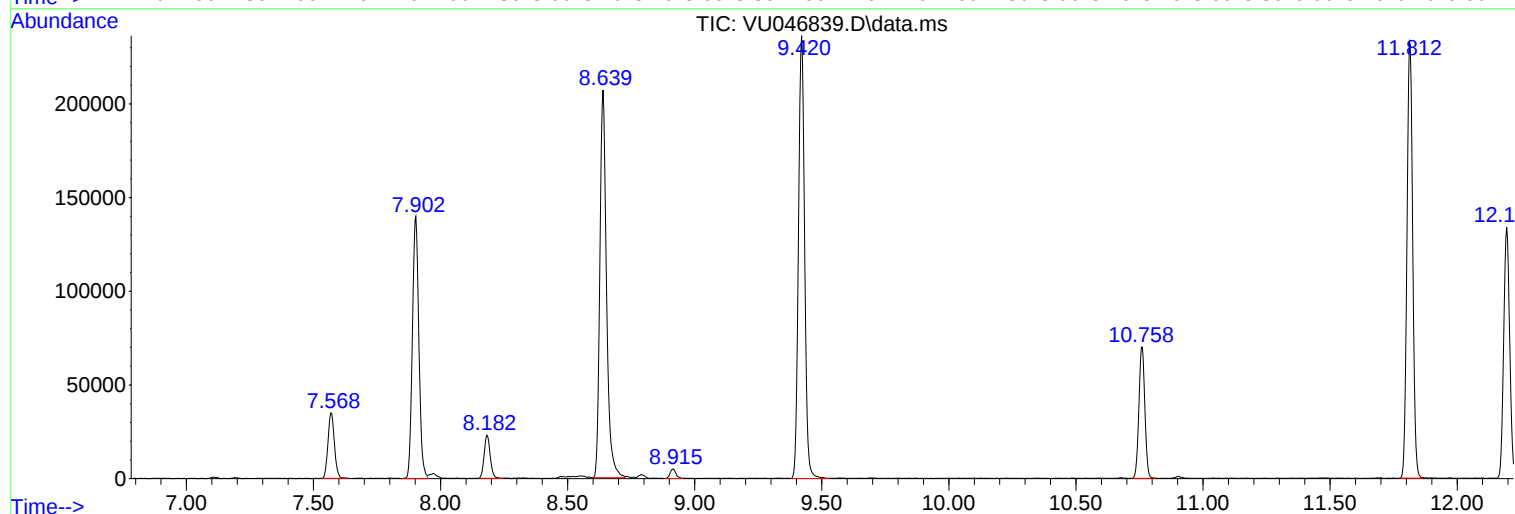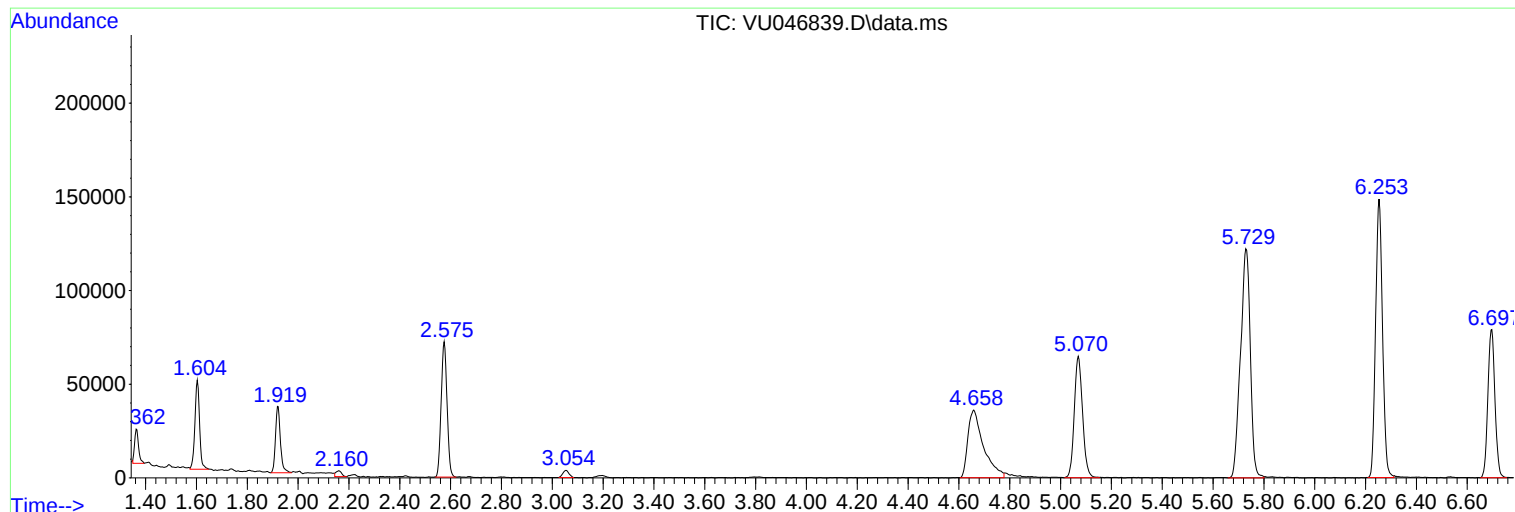

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046839.D
Acq On : 26 Jan 2022 12:32
Operator : SY/MD
Sample : N1260-02 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046839.D
Acq On : 26 Jan 2022 12:32
Operator : SY/MD
Sample : N1260-02 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc