

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
 Data File : VU046840.D
 Acq On : 26 Jan 2022 12:57
 Operator : SY/MD
 Sample : N1260-01 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFX3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046840.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	97	rBV	52824	60986	12.85%	1.794%
2	1.919	171	180	203	rVB	43154	60515	12.75%	1.780%
3	2.575	372	384	401	rBV	87732	143273	30.18%	4.215%
4	3.054	524	533	545	rVB3	3364	5616	1.18%	0.165%
5	4.652	1015	1030	1081	rBV	42067	192673	40.59%	5.669%
6	5.070	1142	1160	1181	rBV	78356	177347	37.36%	5.218%
7	5.729	1344	1365	1385	rBV2	154781	402432	84.78%	11.840%
8	6.253	1513	1528	1550	rBV	120862	228458	48.13%	6.722%
9	6.693	1650	1665	1685	rBV	94548	185582	39.10%	5.460%
10	7.568	1925	1937	1955	rBV	42757	75648	15.94%	2.226%
11	7.899	2027	2040	2056	rBV	175113	303224	63.88%	8.921%
12	8.182	2118	2128	2144	rBV	28189	46350	9.76%	1.364%
13	8.639	2257	2270	2302	rBV	253718	474660	100.00%	13.965%
14	8.790	2310	2317	2331	rVB6	4014	6600	1.39%	0.194%
15	8.912	2346	2355	2371	rVB3	3901	5952	1.25%	0.175%
16	9.420	2500	2513	2535	rBV	192053	320521	67.53%	9.430%
17	10.758	2918	2929	2944	rBV	85601	139817	29.46%	4.114%
18	11.812	3246	3257	3273	rBV	186459	292259	61.57%	8.599%
19	12.195	3362	3376	3395	rBV	167174	270527	56.99%	7.959%
20	12.889	3583	3592	3601	rBV5	4810	6468	1.36%	0.190%




Sum of corrected areas: 3398908

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046840.D
Acq On : 26 Jan 2022 12:57
Operator : SY/MD
Sample : N1260-01 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

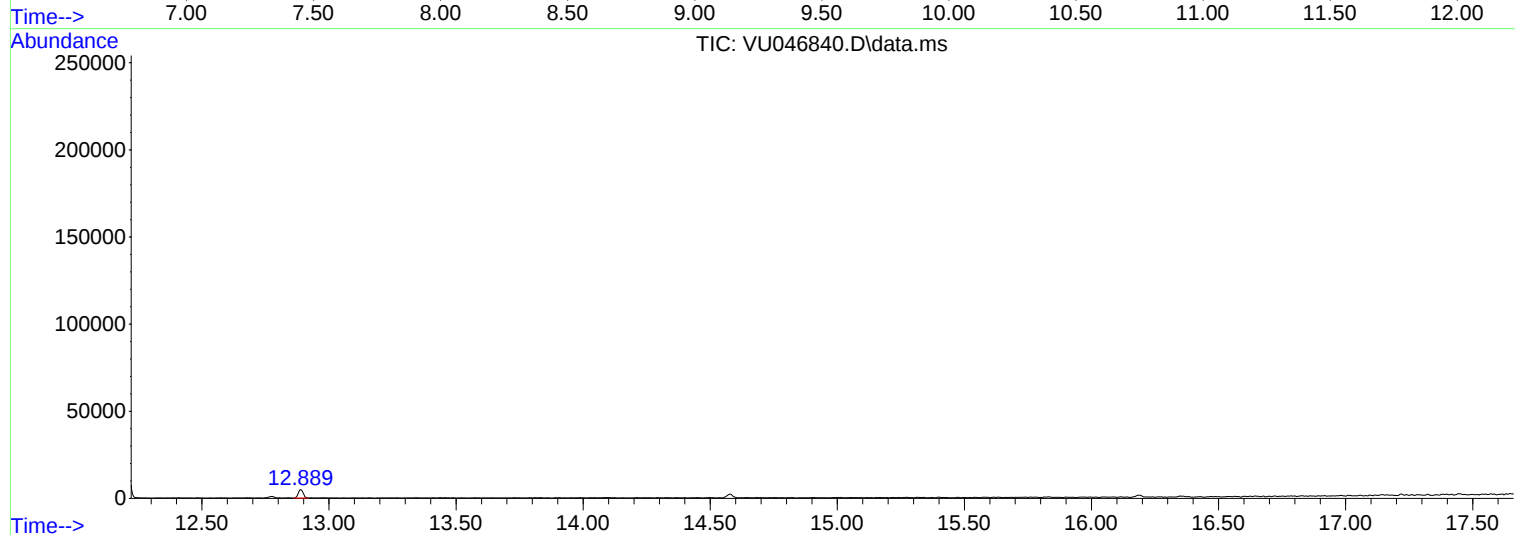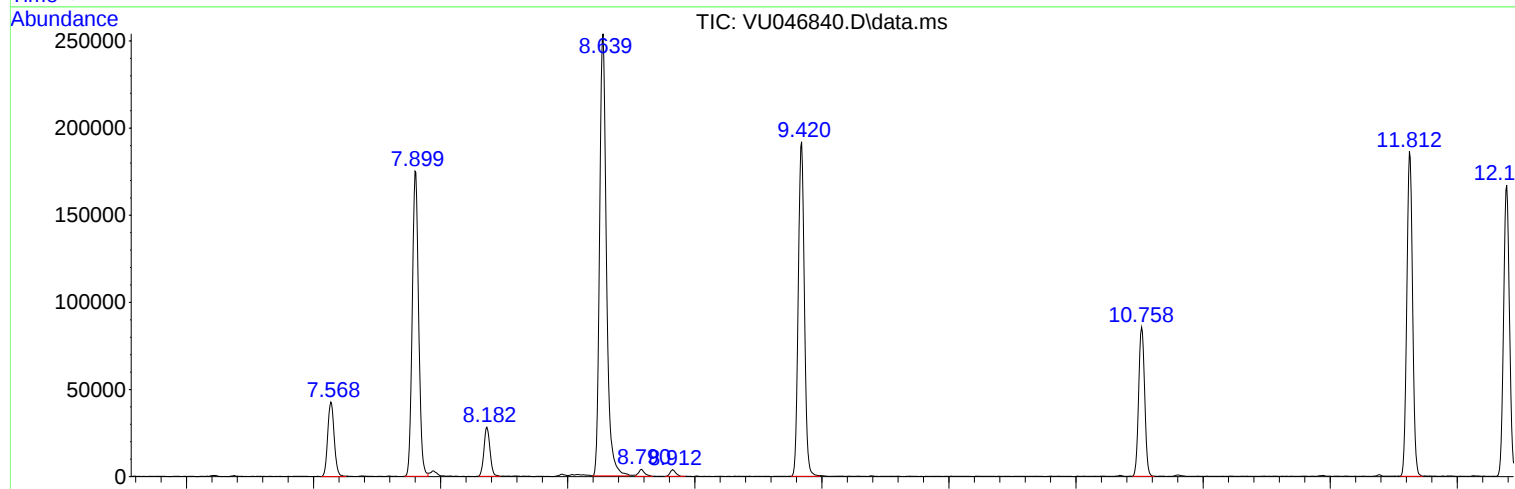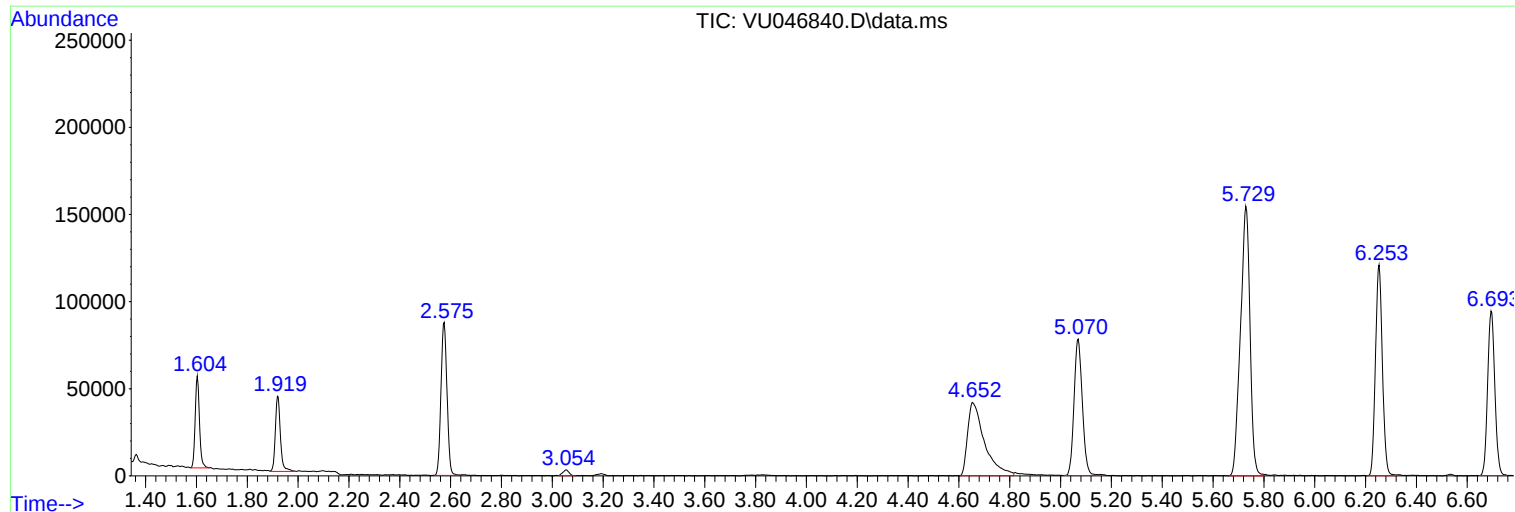

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046840.D
Acq On : 26 Jan 2022 12:57
Operator : SY/MD
Sample : N1260-01 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046840.D
Acq On : 26 Jan 2022 12:57
Operator : SY/MD
Sample : N1260-01 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc