

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
 Data File : VU046851.D
 Acq On : 26 Jan 2022 17:51
 Operator : SY/MD
 Sample : N1277-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COVID7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	15	rVB2	3943	4382	1.01%	0.136%
2	1.604	74	82	93	rVB	46896	52420	12.10%	1.631%
3	1.919	171	180	202	rBV	40430	54714	12.63%	1.702%
4	2.575	372	384	397	rBV	78100	126111	29.12%	3.924%
5	4.642	1012	1027	1064	rBV	56765	179588	41.46%	5.588%
6	5.067	1144	1159	1179	rBV	73766	162926	37.62%	5.070%
7	5.729	1343	1365	1390	rBV2	143816	377609	87.18%	11.750%
8	6.253	1512	1528	1550	rBV	121724	232421	53.66%	7.232%
9	6.694	1650	1665	1686	rBV	90269	174802	40.36%	5.439%
10	7.568	1923	1937	1953	rBV2	41724	71874	16.59%	2.236%
11	7.899	2027	2040	2057	rBV	161430	285136	65.83%	8.872%
12	8.182	2117	2128	2143	rBV2	26981	44267	10.22%	1.377%
13	8.475	2206	2219	2229	rBV2	3464	7243	1.67%	0.225%
14	8.636	2257	2269	2294	rBV	246192	433114	100.00%	13.477%
15	9.420	2501	2513	2535	rBV	188381	317099	73.21%	9.867%
16	10.758	2918	2929	2944	rVB	78431	125989	29.09%	3.920%
17	10.896	2960	2972	2982	rVB2	2968	4779	1.10%	0.149%
18	11.812	3242	3257	3275	rVB	186533	292986	67.65%	9.117%
19	12.060	3325	3334	3346	rBV3	6026	9358	2.16%	0.291%
20	12.195	3363	3376	3395	rVB	158456	256949	59.33%	7.995%




Sum of corrected areas: 3213767

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046851.D
Acq On : 26 Jan 2022 17:51
Operator : SY/MD
Sample : N1277-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0VD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

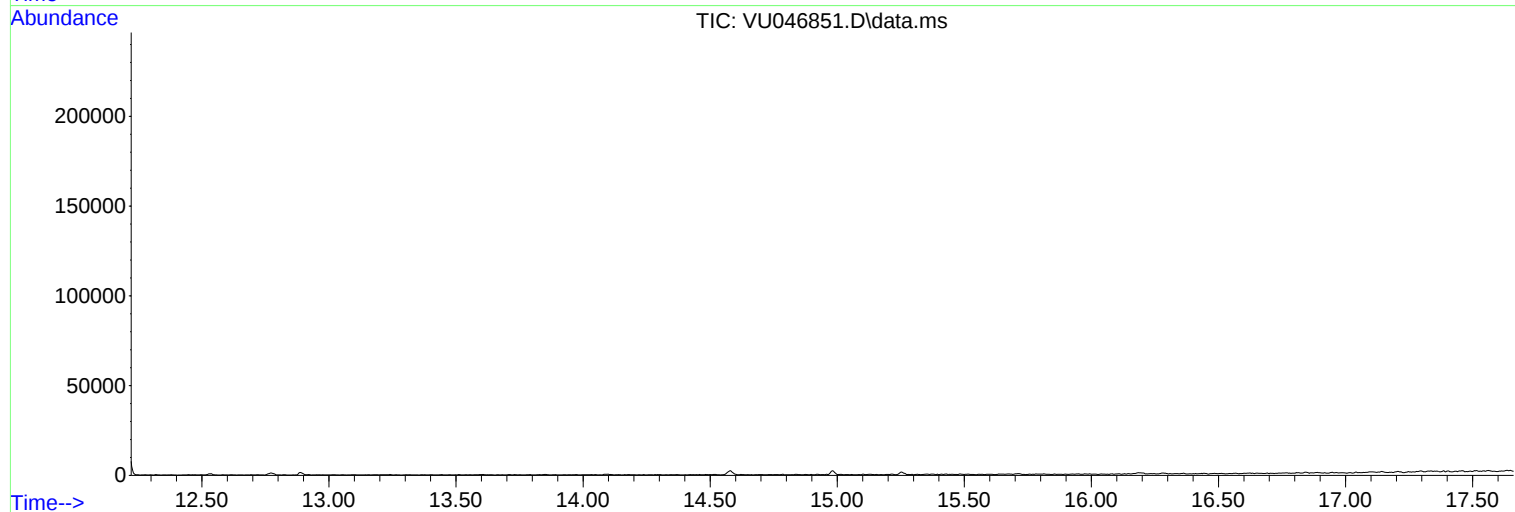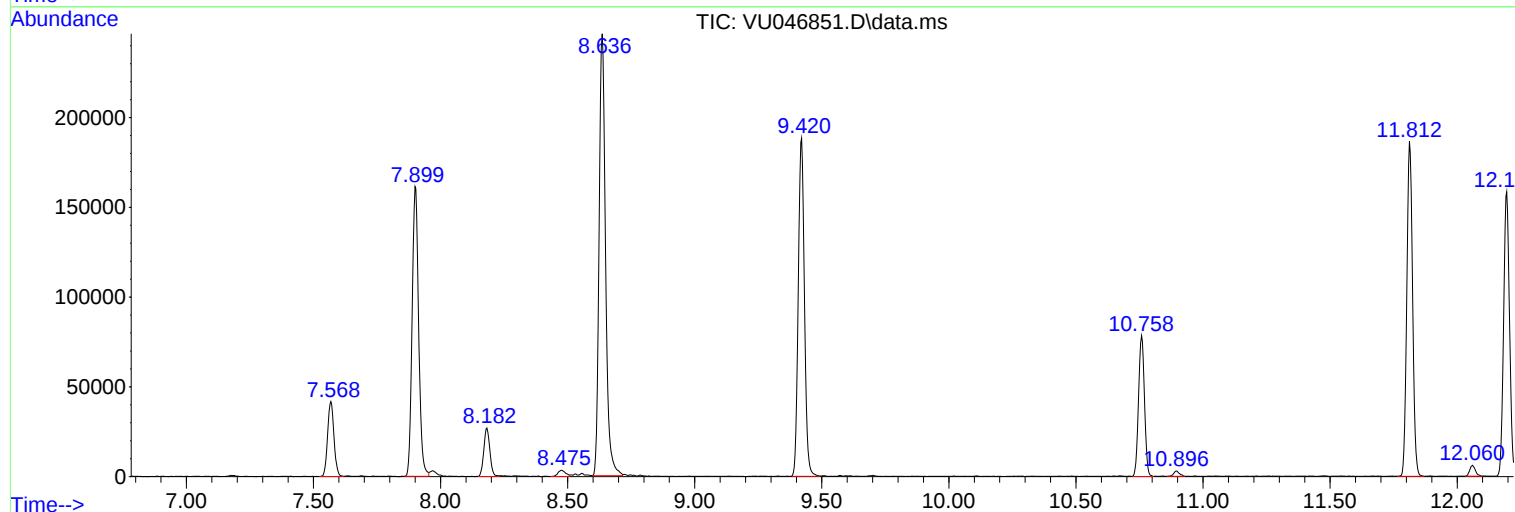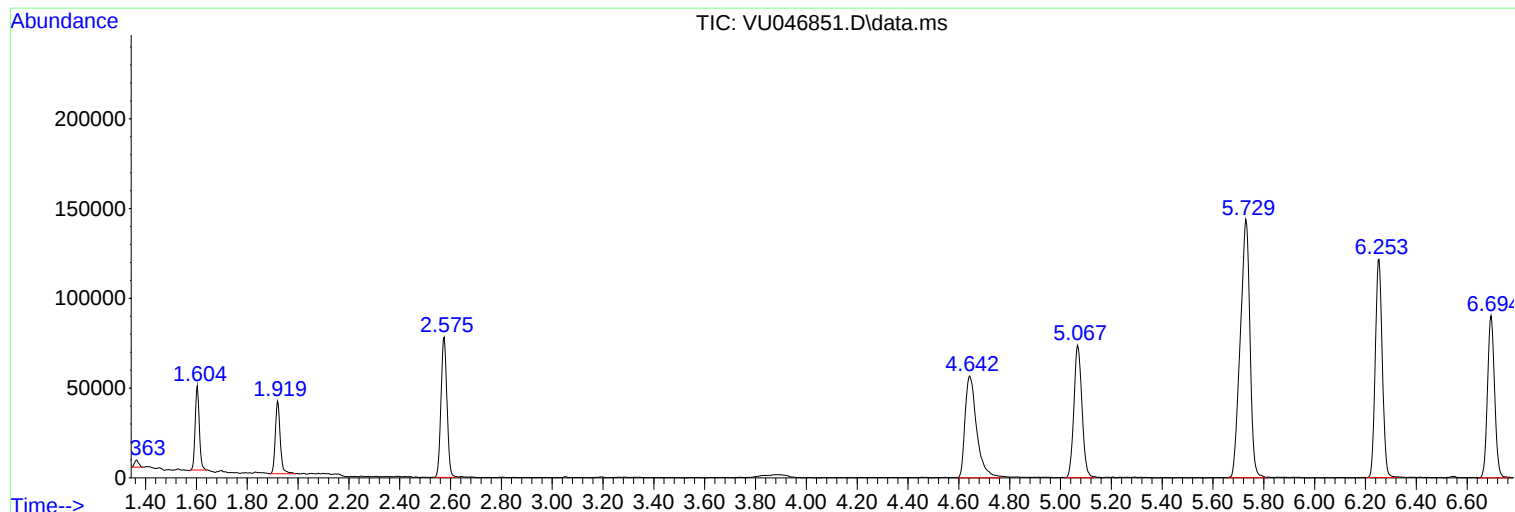

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046851.D
Acq On : 26 Jan 2022 17:51
Operator : SY/MD
Sample : N1277-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0VD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046851.D
Acq On : 26 Jan 2022 17:51
Operator : SY/MD
Sample : N1277-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0VD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
