

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
 Data File : VU046853.D
 Acq On : 26 Jan 2022 18:40
 Operator : SY/MD
 Sample : N1277-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0VD6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	97	rVB	49230	57002	12.31%	1.723%
2	1.735	116	123	132	rVB	6260	8430	1.82%	0.255%
3	1.919	171	180	194	rBV	42691	55376	11.96%	1.674%
4	2.575	372	384	398	rBV	81742	131883	28.48%	3.986%
5	4.652	1014	1030	1068	rBV2	43509	186148	40.19%	5.626%
6	5.067	1141	1159	1181	rBV	76768	169429	36.58%	5.121%
7	5.729	1345	1365	1390	rBV3	150958	391771	84.59%	11.841%
8	6.253	1514	1528	1547	rBV	120636	228363	49.31%	6.902%
9	6.693	1652	1665	1681	rBV2	91854	178323	38.50%	5.390%
10	7.568	1925	1937	1952	rBV	42990	74920	16.18%	2.264%
11	7.899	2028	2040	2058	rBV	165630	295348	63.77%	8.927%
12	8.182	2116	2128	2140	rBV	27697	46480	10.04%	1.405%
13	8.475	2208	2219	2230	rBV4	3865	7833	1.69%	0.237%
14	8.639	2257	2270	2296	rBV	250938	463131	100.00%	13.998%
15	9.420	2498	2513	2533	rBV	184826	316142	68.26%	9.555%
16	10.758	2917	2929	2943	rBV	83572	132245	28.55%	3.997%
17	10.893	2962	2971	2989	rVB	4332	7075	1.53%	0.214%
18	11.812	3245	3257	3274	rBV	176821	282080	60.91%	8.526%
19	12.060	3326	3334	3343	rBV2	8310	12810	2.77%	0.387%
20	12.195	3363	3376	3390	rBV	163493	263801	56.96%	7.973%




Sum of corrected areas: 3308590

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046853.D
Acq On : 26 Jan 2022 18:40
Operator : SY/MD
Sample : N1277-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0VD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

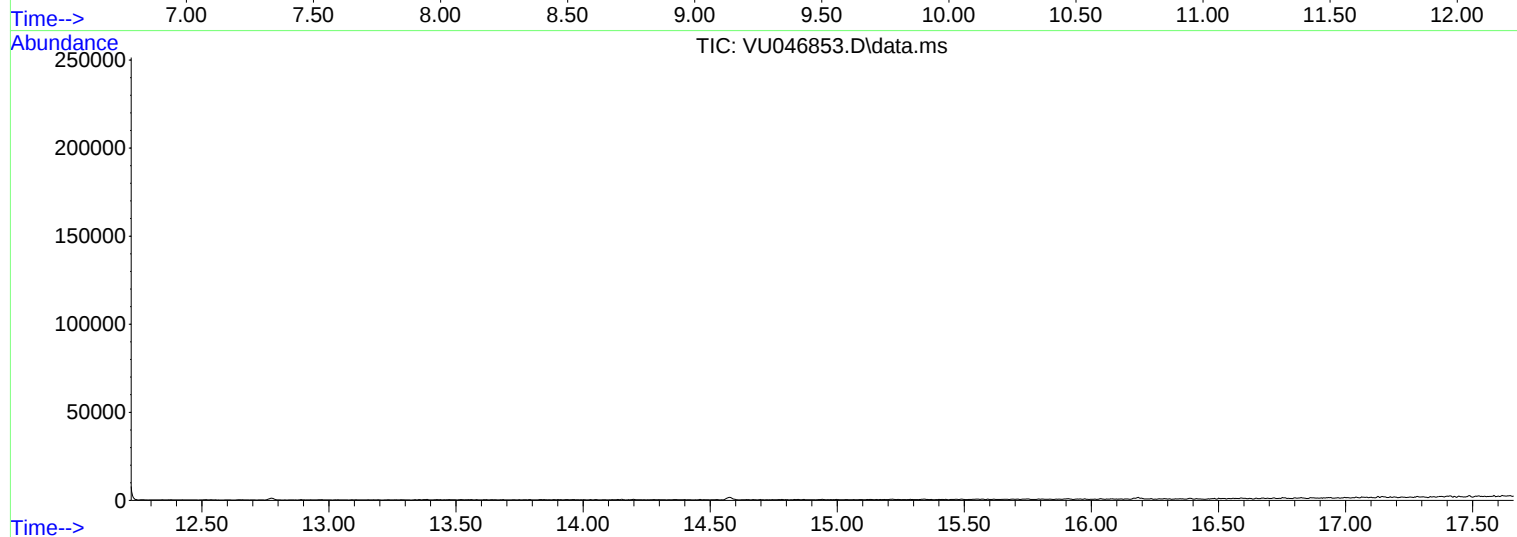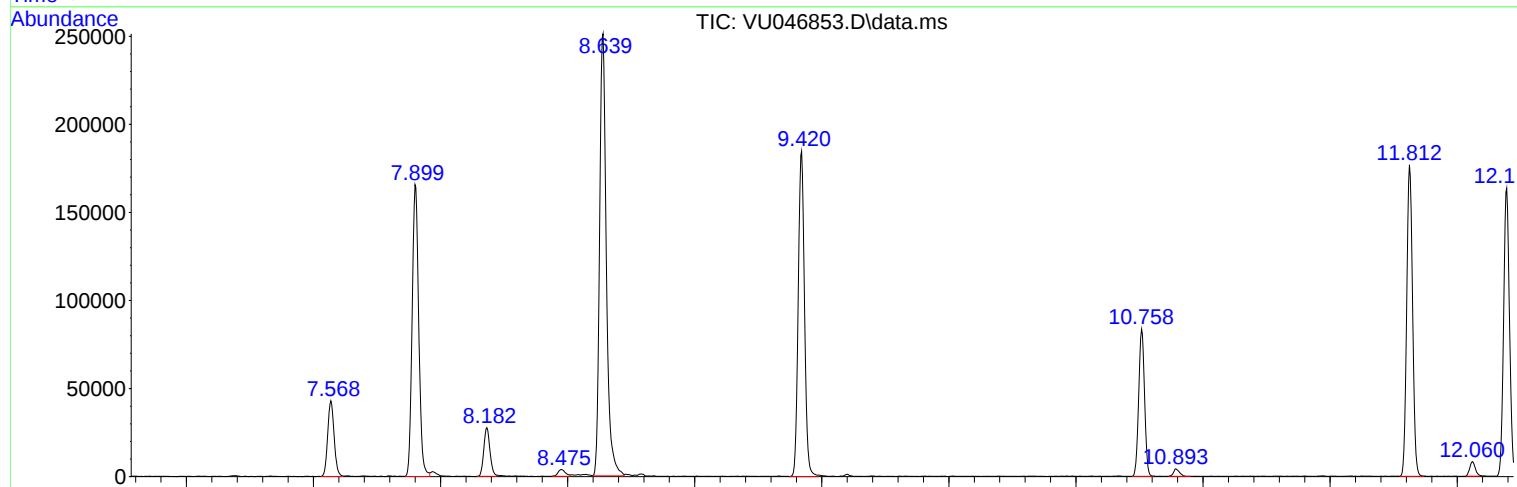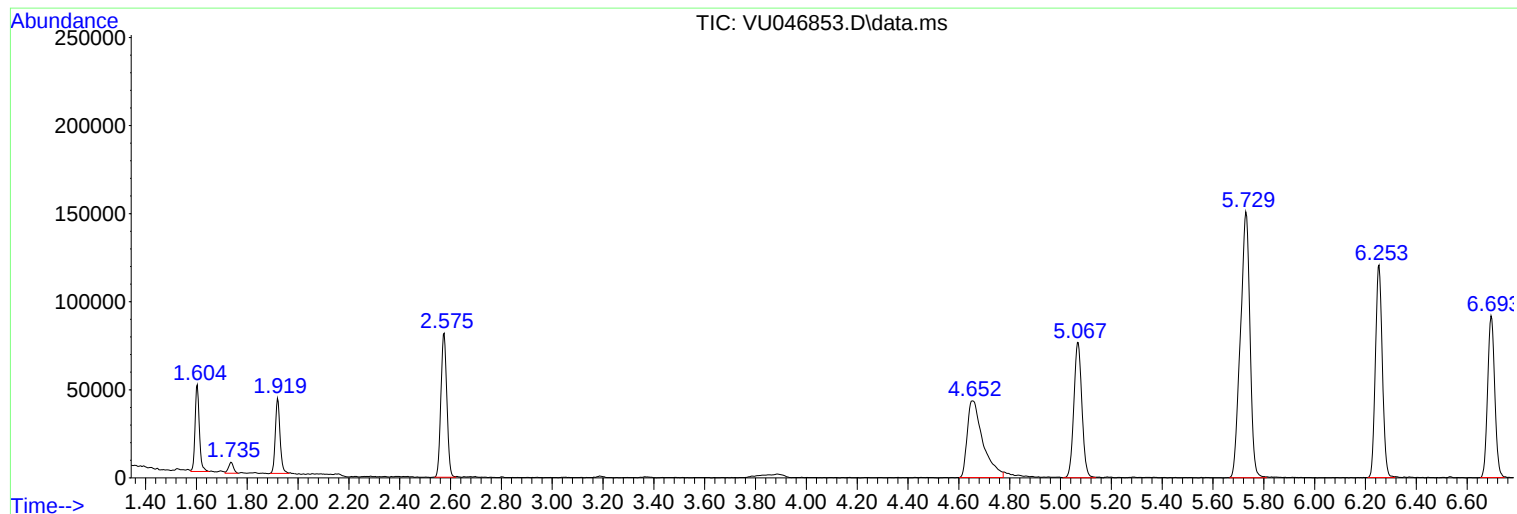

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046853.D
Acq On : 26 Jan 2022 18:40
Operator : SY/MD
Sample : N1277-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0VD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
Data File : VU046853.D
Acq On : 26 Jan 2022 18:40
Operator : SY/MD
Sample : N1277-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0VD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc