


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012622\
 Data File : VU046836.D
 Acq On : 26 Jan 2022 08:58
 Operator : SY/MD
 Sample : BFB047
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB047

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Jan 27 00:12:19 2022

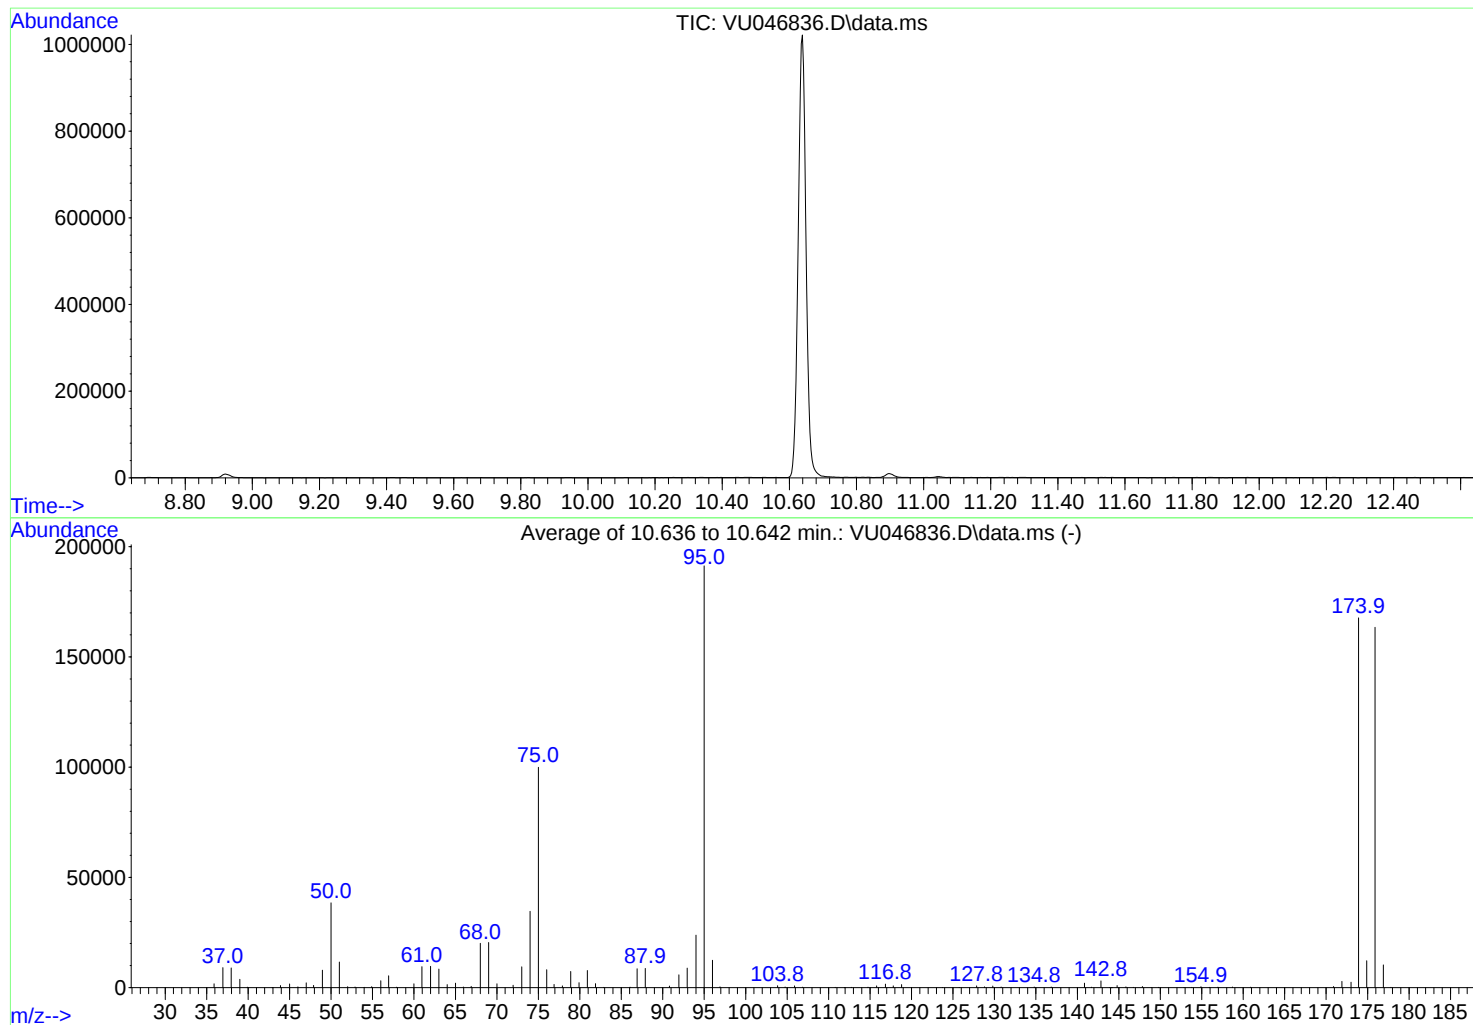

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	38459	PASS
75	95	30	80	52.2	99949	PASS
95	95	100	100	100.0	191317	PASS
96	95	5	9	6.5	12387	PASS
173	174	0.00	2	1.5	2488	PASS
174	95	50	120	87.7	167723	PASS
175	174	5	9	7.3	12217	PASS
176	174	95	101	97.5	163456	PASS
177	176	5	9	6.3	10323	PASS

m/z	Abundance
36.00	281.0
37.90	113.0
39.90	136.0
43.90	389.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047

m/z	Abundance
35.90	2141.0
37.00	9367.0
38.00	9156.0
39.00	4174.0
40.00	325.0
42.90	108.0
43.90	1407.0
45.00	1664.0
46.00	462.0
47.00	2252.0
47.90	1084.0
49.00	8287.0
50.00	39784.0
51.00	11753.0
52.00	471.0
52.90	286.0
54.00	132.0
54.90	484.0
56.00	3290.0
57.00	5683.0
57.90	285.0
60.00	1809.0
61.00	9799.0
62.00	10013.0
63.00	8911.0
64.00	1530.0
65.00	2137.0
66.00	316.0
66.90	565.0
68.00	20672.0
69.00	20976.0
70.00	1685.0
71.90	1206.0
73.00	9380.0
74.00	35512.0
75.00	101400.0
76.00	8405.0
76.90	1493.0
77.90	756.0
78.90	7272.0
79.90	2299.0
80.90	8161.0
81.90	1707.0
82.90	152.0
86.10	248.0
86.90	8732.0
87.90	9032.0
90.80	752.0
91.90	6206.0
92.90	8679.0
94.00	24168.0
95.00	194048.0
96.00	12906.0
96.90	344.0
103.80	897.0
104.70	335.0
105.90	765.0
106.80	204.0
110.80	178.0
111.90	102.0
112.80	212.0
114.80	280.0
115.80	812.0
116.90	1713.0
117.80	758.0
118.80	1398.0
123.70	104.0
127.80	860.0
128.80	410.0
129.80	808.0
130.80	366.0
134.80	357.0
136.80	285.0
140.80	2016.0
141.70	185.0
142.80	3351.0
143.90	153.0
144.80	1066.0
145.80	415.0
146.80	119.0
147.90	597.0
149.70	158.0
152.80	143.0
153.80	171.0
154.90	489.0
155.90	155.0
157.00	203.0
158.70	290.0
160.90	219.0
170.90	541.0
171.90	3080.0
173.00	2455.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047

173.90	164608.0
174.90	12595.0
175.90	162816.0
176.90	10446.0
177.80	184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047

m/z	Abundance
35.90	2117.0
37.00	9324.0
38.00	9488.0
39.00	3822.0
40.00	340.0
43.90	1364.0
45.00	1768.0
46.00	354.0
47.00	2265.0
47.90	1044.0
49.00	8093.0
50.00	39584.0
51.00	11941.0
52.00	469.0
52.90	298.0
54.00	129.0
54.90	441.0
56.00	3209.0
57.00	5539.0
57.90	218.0
60.00	1804.0
61.00	9704.0
62.00	9989.0
63.00	8685.0
64.00	1459.0
65.00	2092.0
66.00	283.0
66.90	592.0
68.00	20712.0
69.00	21216.0
70.00	1799.0
72.00	1078.0
73.00	9804.0
74.00	35688.0
75.00	103264.0
76.00	8354.0
76.90	1541.0
77.90	799.0
78.90	7615.0
79.90	2323.0
80.90	8003.0
81.90	1813.0
82.90	153.0
86.10	240.0
86.90	8700.0
87.90	9151.0
90.80	742.0
91.90	5998.0
93.00	9162.0
94.00	24552.0
95.00	197376.0
96.00	12731.0
96.90	355.0
103.80	873.0
104.80	306.0
105.90	802.0
106.90	226.0
110.80	180.0
112.70	163.0
114.70	258.0
115.80	837.0
116.90	1693.0
117.80	870.0
118.80	1473.0
123.80	101.0
125.70	158.0
127.80	864.0
128.80	369.0
129.80	772.0
130.80	323.0
134.80	324.0
136.90	286.0
140.90	2082.0
141.70	237.0
142.80	3172.0
144.10	111.0
144.80	963.0
145.80	389.0
146.80	161.0
147.90	527.0
148.90	122.0
149.80	163.0
152.90	103.0
153.80	203.0
154.90	483.0
155.90	183.0
156.90	268.0
158.70	284.0
160.90	229.0
170.90	536.0
171.90	2950.0
173.00	2608.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047

173.90	172928.0
174.90	12615.0
175.90	168960.0
176.90	10637.0
177.80	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047

m/z	Abundance
35.90	1858.0
36.90	8577.0
38.00	8537.0
39.00	3289.0
39.90	312.0
43.90	1298.0
45.00	1664.0
46.00	207.0
47.00	1964.0
47.90	1029.0
48.90	7329.0
50.00	36008.0
51.00	11265.0
52.00	411.0
52.90	276.0
54.00	101.0
54.90	393.0
56.00	2875.0
56.90	4969.0
57.90	133.0
60.00	1656.0
60.90	9142.0
62.00	9055.0
63.00	7718.0
64.00	1281.0
65.00	1890.0
65.90	214.0
66.90	555.0
68.00	18896.0
69.00	19264.0
70.00	1738.0
71.90	980.0
73.00	9146.0
74.00	32712.0
75.00	95184.0
76.00	7558.0
76.90	1257.0
77.90	832.0
78.90	7049.0
79.90	2140.0
80.90	7239.0
81.90	1851.0
82.90	134.0
86.00	268.0
86.90	8180.0
87.90	7991.0
90.80	710.0
92.00	5270.0
93.00	8791.0
94.00	22640.0
95.00	182528.0
96.00	11525.0
96.90	331.0
103.90	811.0
104.80	251.0
105.90	790.0
106.90	220.0
110.80	173.0
112.70	129.0
114.80	215.0
115.80	705.0
116.80	1473.0
117.80	842.0
118.80	1351.0
125.80	163.0
127.90	746.0
128.80	350.0
129.80	618.0
130.80	256.0
134.80	274.0
136.90	287.0
140.90	2007.0
141.70	277.0
142.90	2628.0
144.80	805.0
145.90	311.0
146.70	172.0
147.80	388.0
148.90	122.0
149.90	175.0
153.80	173.0
154.90	445.0
155.90	146.0
156.90	318.0
158.70	247.0
160.90	213.0
170.90	458.0
171.90	2542.0
173.00	2401.0
173.90	165632.0
174.90	11442.0
175.90	158592.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047

176.90	9887.0
177.80	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047