

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
 Data File : VU046889.D
 Acq On : 28 Jan 2022 13:42
 Operator : SY/MD
 Sample : N1273-04DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HK3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046889.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	97	rVB	43343	51055	9.52%	1.129%
2	1.919	171	180	194	rBV	40015	52760	9.83%	1.167%
3	2.581	372	386	406	rBV3	150317	290736	54.19%	6.430%
4	3.877	775	789	804	rVB2	5065	10988	2.05%	0.243%
5	4.668	1015	1035	1065	rBV2	75293	271813	50.66%	6.011%
6	5.066	1144	1159	1179	rBV	76020	169533	31.60%	3.749%
7	5.729	1344	1365	1383	rBV2	145414	381870	71.17%	8.445%
8	6.253	1514	1528	1553	rBV	120543	230158	42.90%	5.090%
9	6.546	1604	1619	1642	rBV	252075	469748	87.55%	10.389%
10	6.693	1652	1665	1686	rBV	94158	183145	34.14%	4.050%
11	7.568	1924	1937	1951	rBV2	41774	73210	13.65%	1.619%
12	7.899	2028	2040	2060	rBV	151478	273697	51.01%	6.053%
13	8.182	2117	2128	2145	rBV	26297	43977	8.20%	0.973%
14	8.555	2232	2244	2259	rBV	313222	536524	100.00%	11.865%
15	8.639	2259	2270	2304	rVB	252631	498160	92.85%	11.017%
16	9.420	2501	2513	2533	rBV	184863	319353	59.52%	7.063%
17	10.758	2917	2929	2945	rVB	85081	139284	25.96%	3.080%
18	11.812	3243	3257	3275	rBV	173669	279504	52.10%	6.181%
19	12.195	3363	3376	3392	rBV	152746	246291	45.90%	5.447%




Sum of corrected areas: 4521806

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046889.D
Acq On : 28 Jan 2022 13:42
Operator : SY/MD
Sample : N1273-04DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HK3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

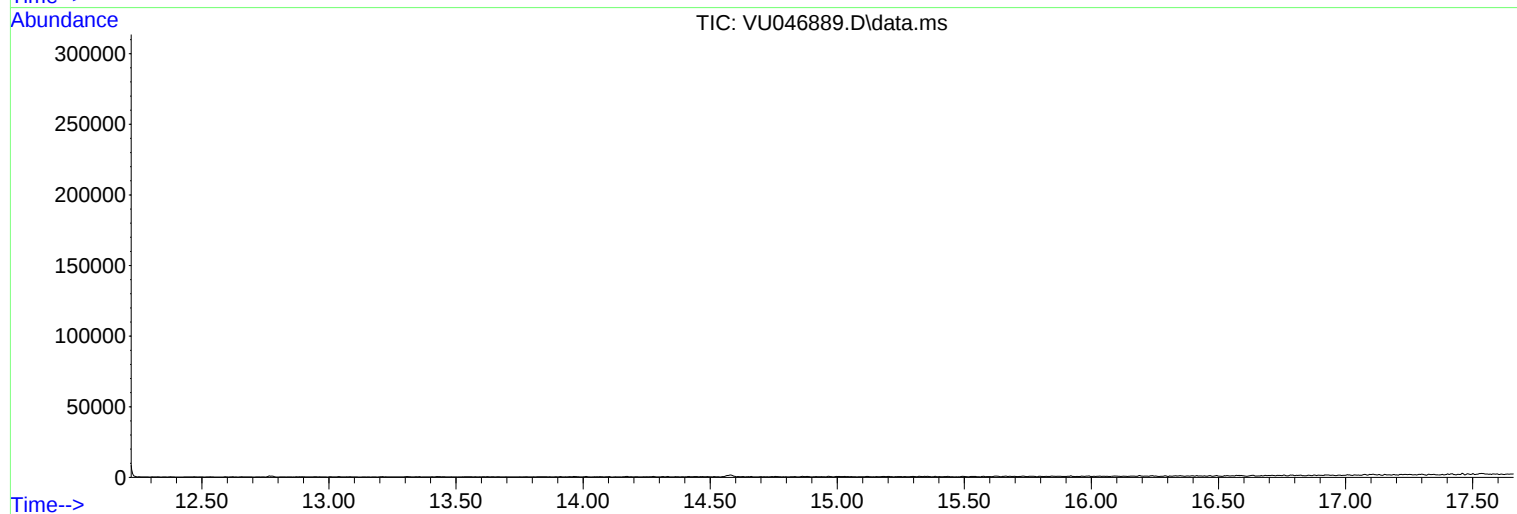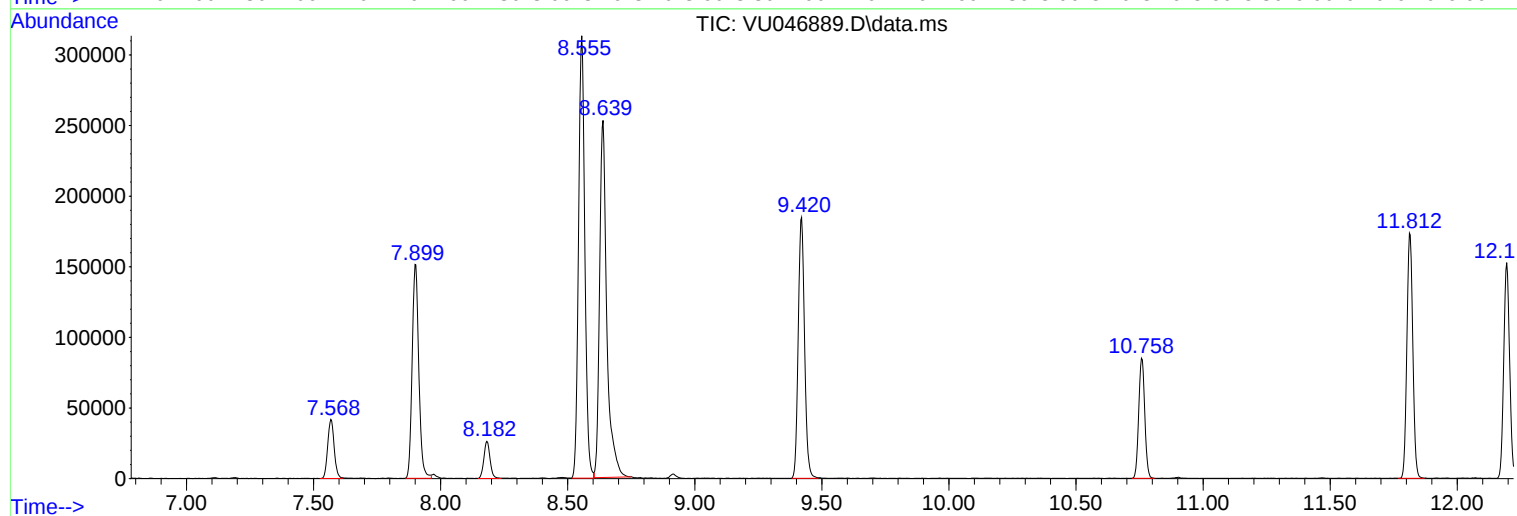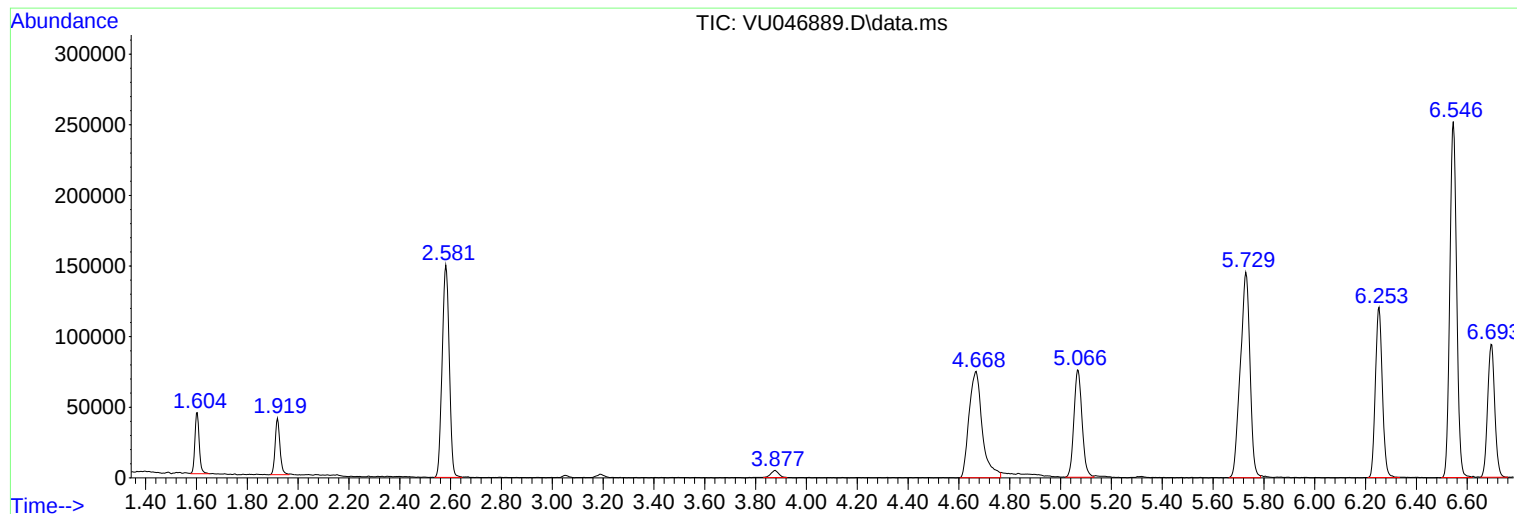

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046889.D
Acq On : 28 Jan 2022 13:42
Operator : SY/MD
Sample : N1273-04DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HK3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046889.D
Acq On : 28 Jan 2022 13:42
Operator : SY/MD
Sample : N1273-04DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HK3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
