

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
 Data File : VU046892.D
 Acq On : 28 Jan 2022 14:56
 Operator : SY/MD
 Sample : N1273-06DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HK5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046892.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	14	rVB	5328	4965	1.02%	0.139%
2	1.604	74	82	96	rBV2	72242	89453	18.30%	2.499%
3	1.919	171	180	194	rBV	40074	53710	10.99%	1.501%
4	2.572	371	383	395	rBV	74965	122595	25.07%	3.425%
5	3.880	777	790	801	rVB	3471	7124	1.46%	0.199%
6	4.652	1013	1030	1067	rBV2	57066	213187	43.60%	5.956%
7	5.067	1140	1159	1184	rVB	76705	171160	35.01%	4.782%
8	5.729	1345	1365	1387	rBV2	143069	376404	76.99%	10.517%
9	6.253	1514	1528	1548	rBV	111905	213904	43.75%	5.977%
10	6.546	1608	1619	1634	rVB2	19900	35328	7.23%	0.987%
11	6.694	1651	1665	1685	rBV	92481	181218	37.06%	5.063%
12	7.568	1925	1937	1951	rBV	41638	70587	14.44%	1.972%
13	7.899	2028	2040	2057	rBV	145278	263781	53.95%	7.370%
14	8.179	2117	2127	2144	rBV	26224	43990	9.00%	1.229%
15	8.555	2231	2244	2258	rBV	180818	307772	62.95%	8.599%
16	8.636	2258	2269	2297	rVB	268180	488930	100.00%	13.661%
17	9.420	2500	2513	2529	rBV	175024	298025	60.95%	8.327%
18	10.758	2917	2929	2944	rBV	87476	137537	28.13%	3.843%
19	11.812	3245	3257	3272	rBV	162810	259407	53.06%	7.248%
20	12.195	3364	3376	3395	rVB	147914	240007	49.09%	6.706%




Sum of corrected areas: 3579084

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046892.D
Acq On : 28 Jan 2022 14:56
Operator : SY/MD
Sample : N1273-06DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HK5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

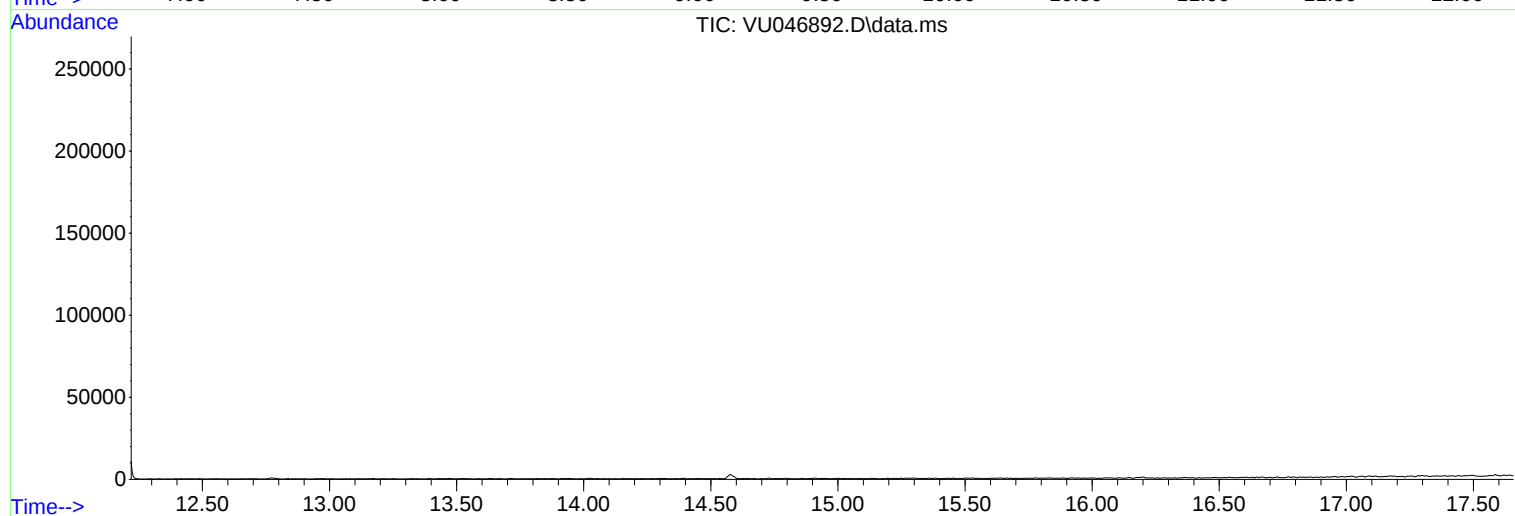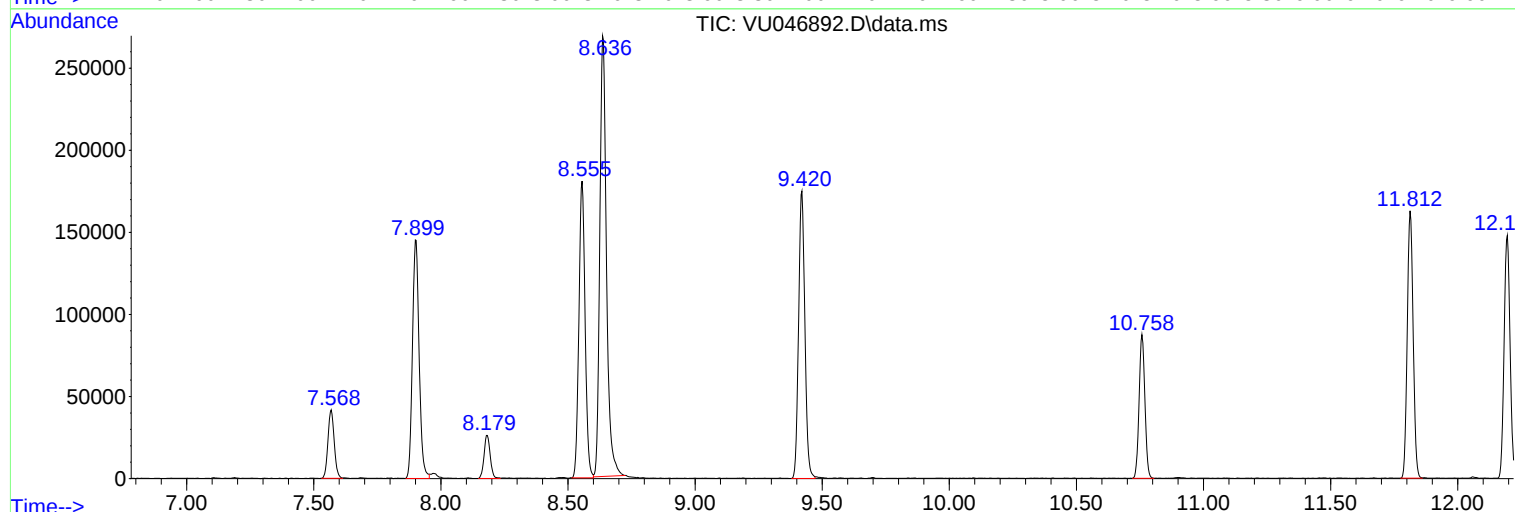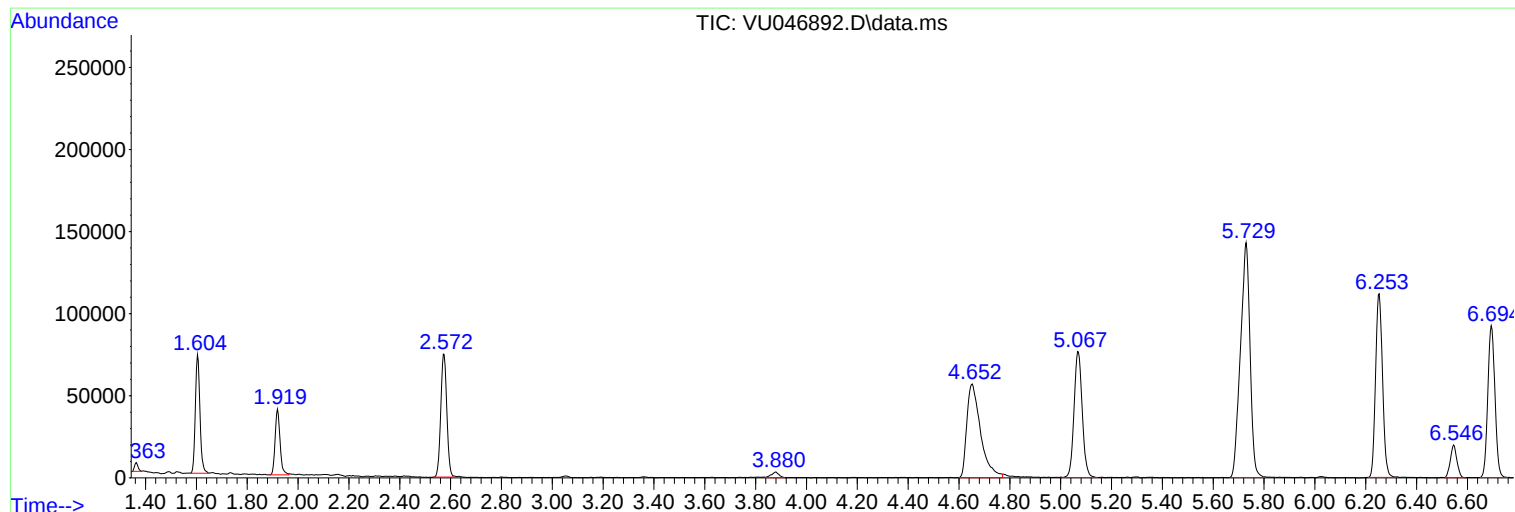

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046892.D
Acq On : 28 Jan 2022 14:56
Operator : SY/MD
Sample : N1273-06DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HK5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046892.D
Acq On : 28 Jan 2022 14:56
Operator : SY/MD
Sample : N1273-06DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HK5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc