

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
 Data File : VU046899.D
 Acq On : 28 Jan 2022 17:48
 Operator : SY/MD
 Sample : N1273-13DL 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HL1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	92	rBV	39297	43850	6.47%	1.067%
2	1.919	171	180	199	rVB	37571	50414	7.44%	1.227%
3	2.575	371	384	399	rBV3	78750	140252	20.68%	3.414%
4	4.668	1014	1035	1082	rBV3	109424	371841	54.84%	9.051%
5	5.070	1144	1160	1190	rVB	74303	166727	24.59%	4.058%
6	5.321	1225	1238	1250	rVB3	4659	10502	1.55%	0.256%
7	5.729	1341	1365	1385	rBV2	137379	363961	53.68%	8.859%
8	6.253	1514	1528	1552	rBV2	111561	213359	31.47%	5.193%
9	6.546	1606	1619	1637	rBV	73237	135384	19.97%	3.295%
10	6.694	1651	1665	1682	rBV	89801	174628	25.75%	4.250%
11	7.568	1926	1937	1951	rBV2	39526	67616	9.97%	1.646%
12	7.902	2027	2041	2058	rBV	136502	253074	37.32%	6.160%
13	8.182	2118	2128	2141	rBV	24804	41267	6.09%	1.004%
14	8.555	2231	2244	2259	rBV	389098	678058	100.00%	16.504%
15	8.639	2259	2270	2299	rVB	251702	478577	70.58%	11.649%
16	9.420	2500	2513	2534	rBV	169724	300572	44.33%	7.316%
17	10.758	2915	2929	2948	rBV	83933	134114	19.78%	3.264%
18	11.812	3245	3257	3276	rVB	155430	254013	37.46%	6.183%
19	12.195	3364	3376	3392	rBV	139847	230221	33.95%	5.604%




Sum of corrected areas: 4108430

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046899.D
Acq On : 28 Jan 2022 17:48
Operator : SY/MD
Sample : N1273-13DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

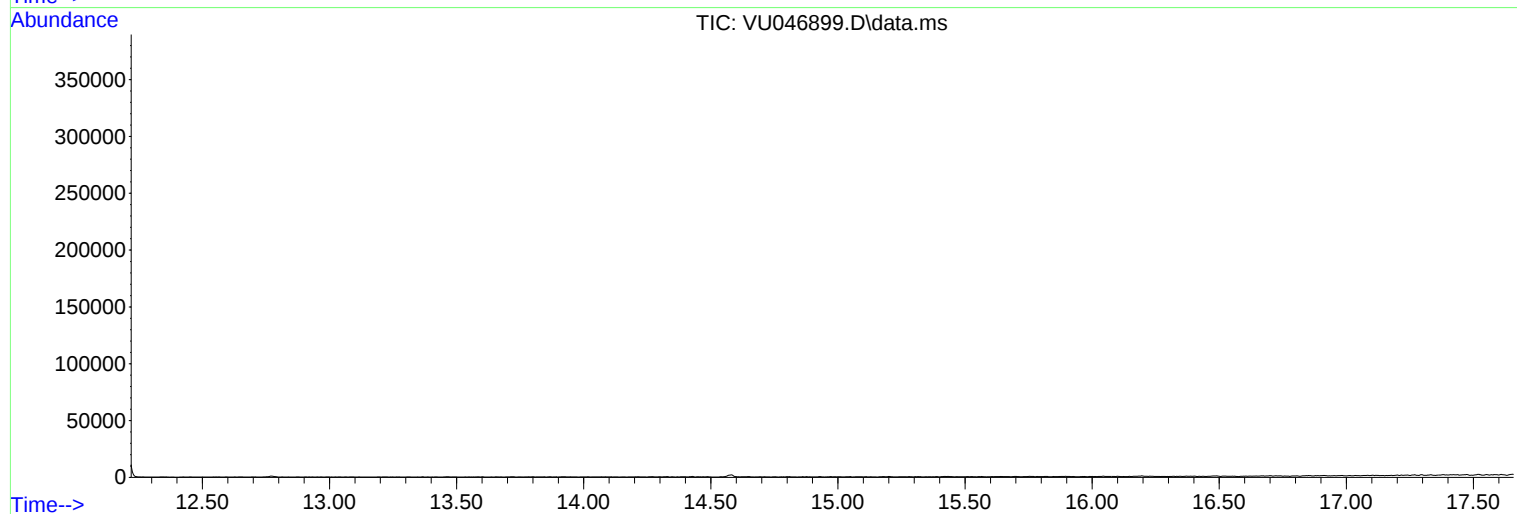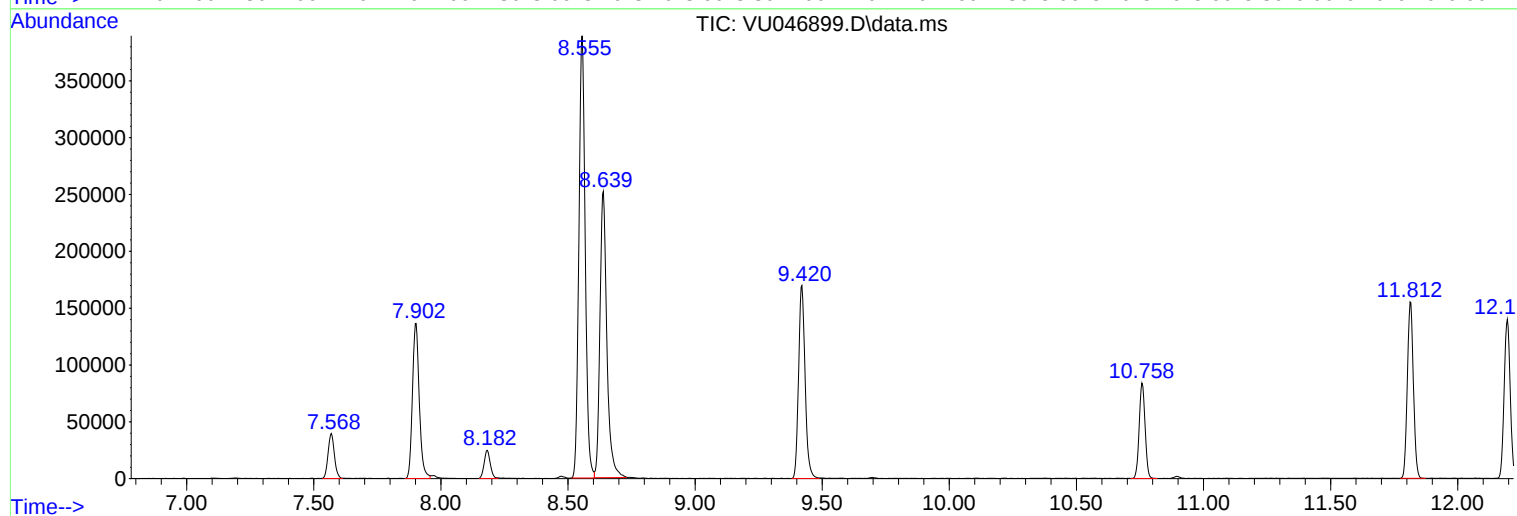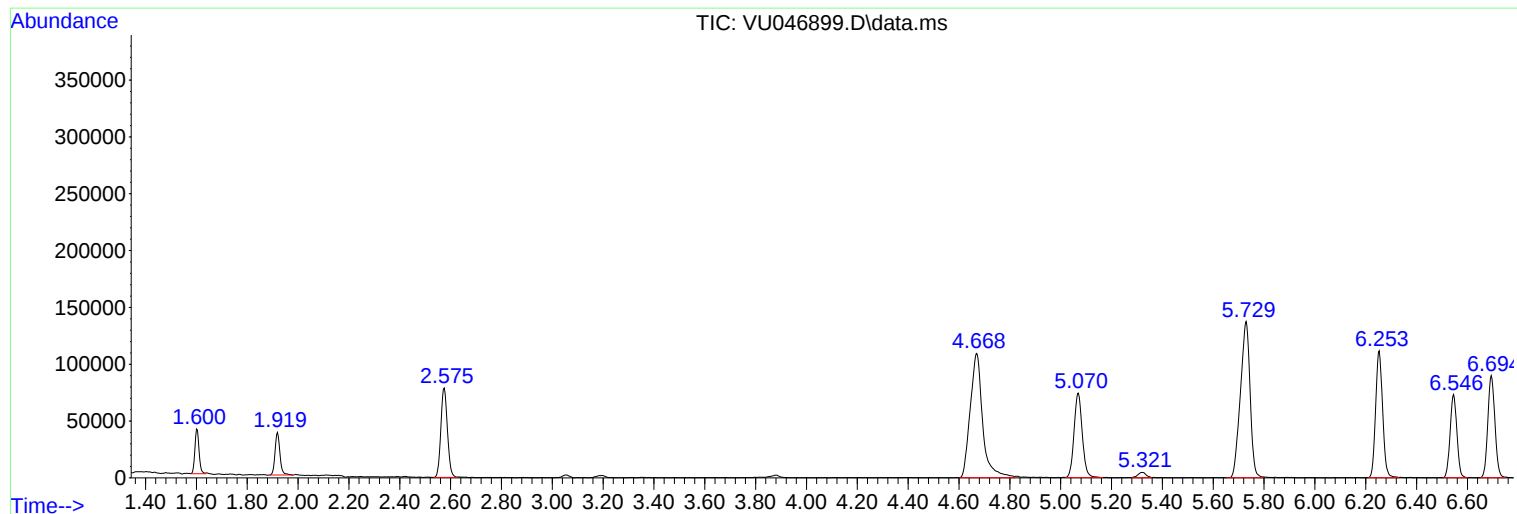

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046899.D
Acq On : 28 Jan 2022 17:48
Operator : SY/MD
Sample : N1273-13DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046899.D
Acq On : 28 Jan 2022 17:48
Operator : SY/MD
Sample : N1273-13DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc