

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
 Data File : VU046900.D
 Acq On : 28 Jan 2022 18:12
 Operator : SY/MD
 Sample : N1273-14DL 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HL2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	96	rVB	38177	44458	7.10%	1.119%
2	1.919	171	180	202	rVB	36387	49138	7.85%	1.237%
3	2.571	372	383	398	rBV2	75926	134987	21.55%	3.397%
4	4.668	1010	1035	1082	rBV2	106528	358436	57.23%	9.021%
5	5.067	1143	1159	1180	rBV2	70577	161180	25.74%	4.056%
6	5.321	1225	1238	1251	rVB4	4760	10026	1.60%	0.252%
7	5.729	1344	1365	1387	rBV2	134214	354836	56.66%	8.930%
8	6.253	1515	1528	1548	rBV	112952	216206	34.52%	5.441%
9	6.546	1607	1619	1634	rVB	70111	129069	20.61%	3.248%
10	6.694	1652	1665	1686	rBV	88734	171802	27.43%	4.324%
11	7.568	1924	1937	1949	rBV	39067	65964	10.53%	1.660%
12	7.902	2028	2041	2057	rBV	134325	242911	38.79%	6.113%
13	8.182	2117	2128	2147	rBV2	23504	39979	6.38%	1.006%
14	8.555	2231	2244	2259	rBV	364521	626298	100.00%	15.762%
15	8.639	2259	2270	2303	rVB	241741	460342	73.50%	11.585%
16	9.420	2500	2513	2536	rBV	171574	300365	47.96%	7.559%
17	10.758	2915	2929	2948	rBV	79025	128977	20.59%	3.246%
18	11.812	3242	3257	3276	rBV	158097	258095	41.21%	6.495%
19	12.195	3364	3376	3394	rVB	135364	220450	35.20%	5.548%




Sum of corrected areas: 3973519

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046900.D
Acq On : 28 Jan 2022 18:12
Operator : SY/MD
Sample : N1273-14DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

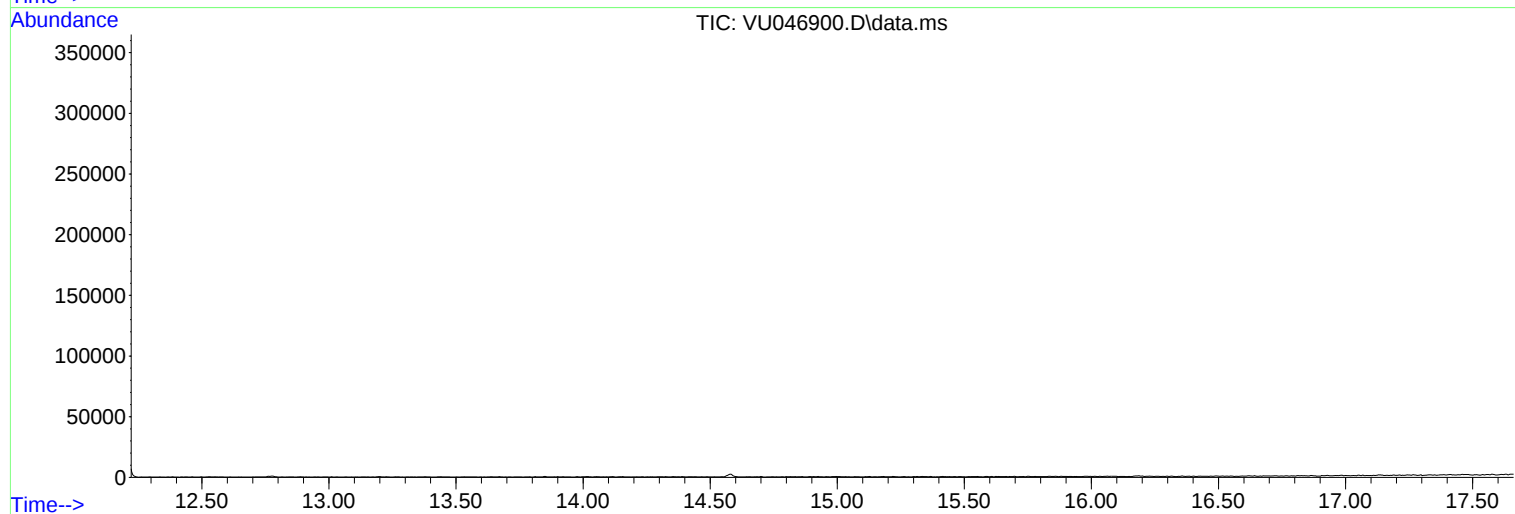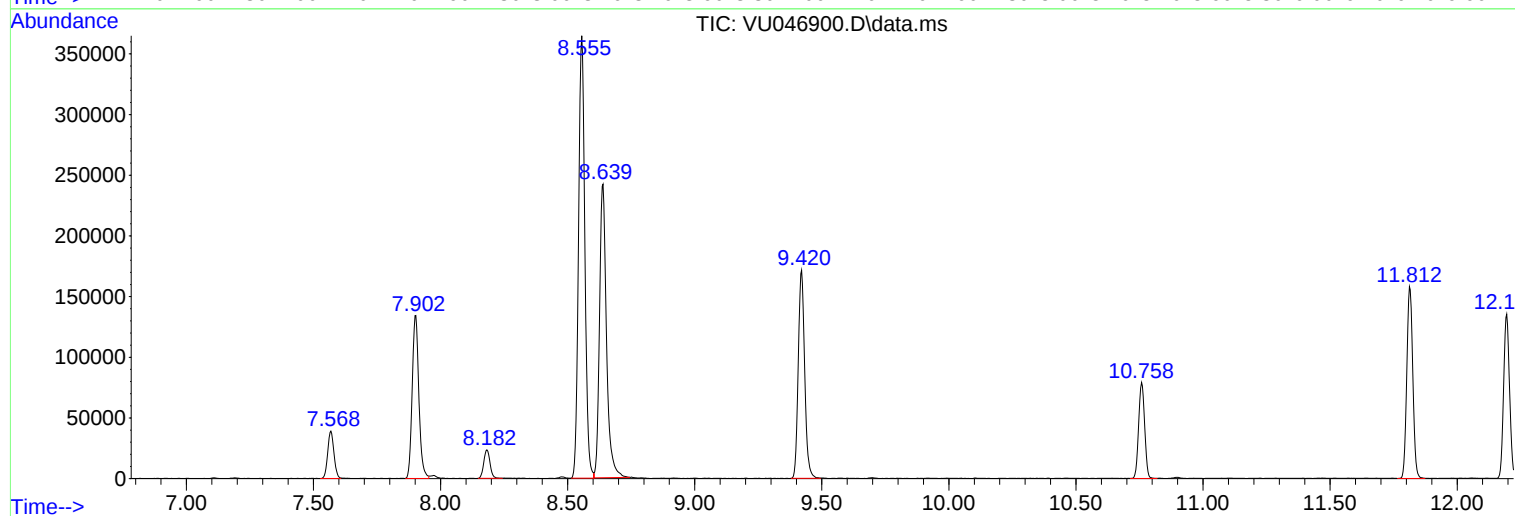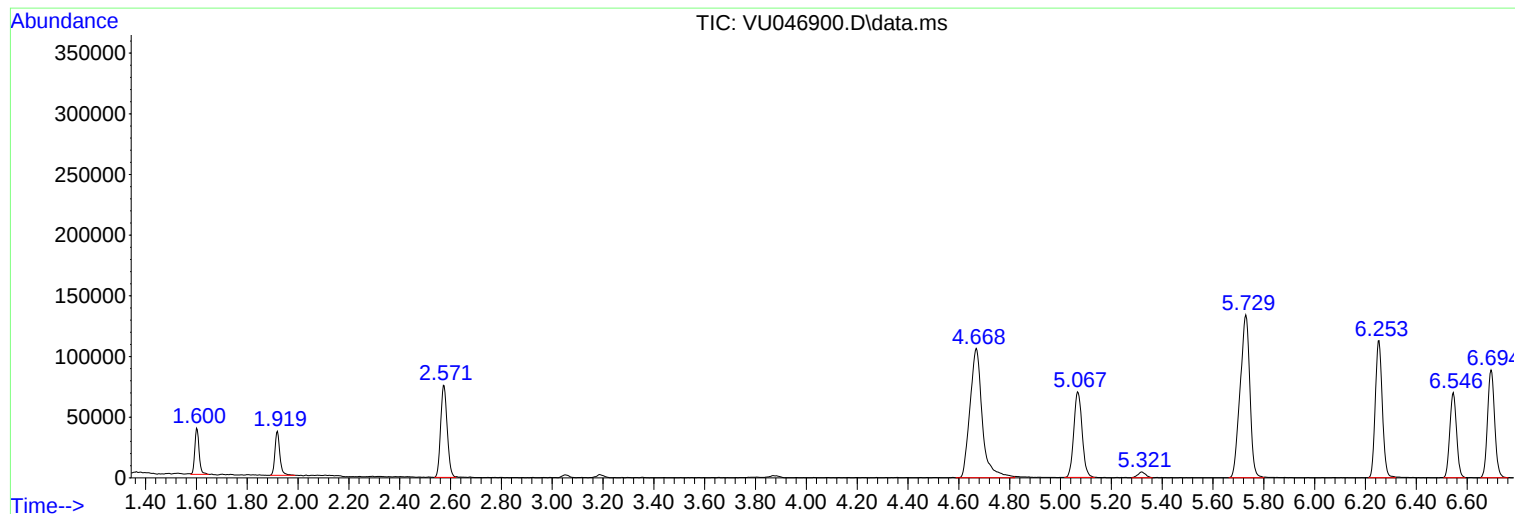

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046900.D
Acq On : 28 Jan 2022 18:12
Operator : SY/MD
Sample : N1273-14DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046900.D
Acq On : 28 Jan 2022 18:12
Operator : SY/MD
Sample : N1273-14DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc