

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
 Data File : VU046902.D
 Acq On : 28 Jan 2022 19:02
 Operator : SY/MD
 Sample : N1273-16 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HL4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU046902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rVB	43020	49225	1.48%	0.518%
2	1.919	171	180	196	rBV	38073	51237	1.54%	0.539%
3	2.585	372	387	411	rBV2	394113	697576	20.97%	7.344%
4	4.665	1013	1034	1069	rBV2	75666	279343	8.40%	2.941%
5	5.067	1144	1159	1184	rVB2	73068	168644	5.07%	1.775%
6	5.321	1219	1238	1258	rBV	89558	199995	6.01%	2.105%
7	5.729	1344	1365	1390	rBV2	136940	362184	10.89%	3.813%
8	6.253	1513	1528	1550	rBV	107022	205887	6.19%	2.167%
9	6.546	1602	1619	1646	rBV	1774698	3326768	100.00%	35.022%
10	6.694	1653	1665	1682	rVB2	93164	184599	5.55%	1.943%
11	7.568	1923	1937	1956	rBV2	40367	70491	2.12%	0.742%
12	7.899	2028	2040	2058	rBV	140489	260096	7.82%	2.738%
13	8.179	2117	2127	2140	rBV2	24769	41503	1.25%	0.437%
14	8.555	2229	2244	2259	rBV	1282940	2203667	66.24%	23.198%
15	8.636	2259	2269	2300	rVB	249602	498637	14.99%	5.249%
16	9.420	2499	2513	2533	rBV	167109	289439	8.70%	3.047%
17	10.758	2917	2929	2943	rBV	81646	133618	4.02%	1.407%
18	11.813	3245	3257	3275	rVB	153494	246040	7.40%	2.590%
19	12.195	3364	3376	3394	rBV	141089	230242	6.92%	2.424%




Sum of corrected areas: 9499191

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046902.D
Acq On : 28 Jan 2022 19:02
Operator : SY/MD
Sample : N1273-16 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

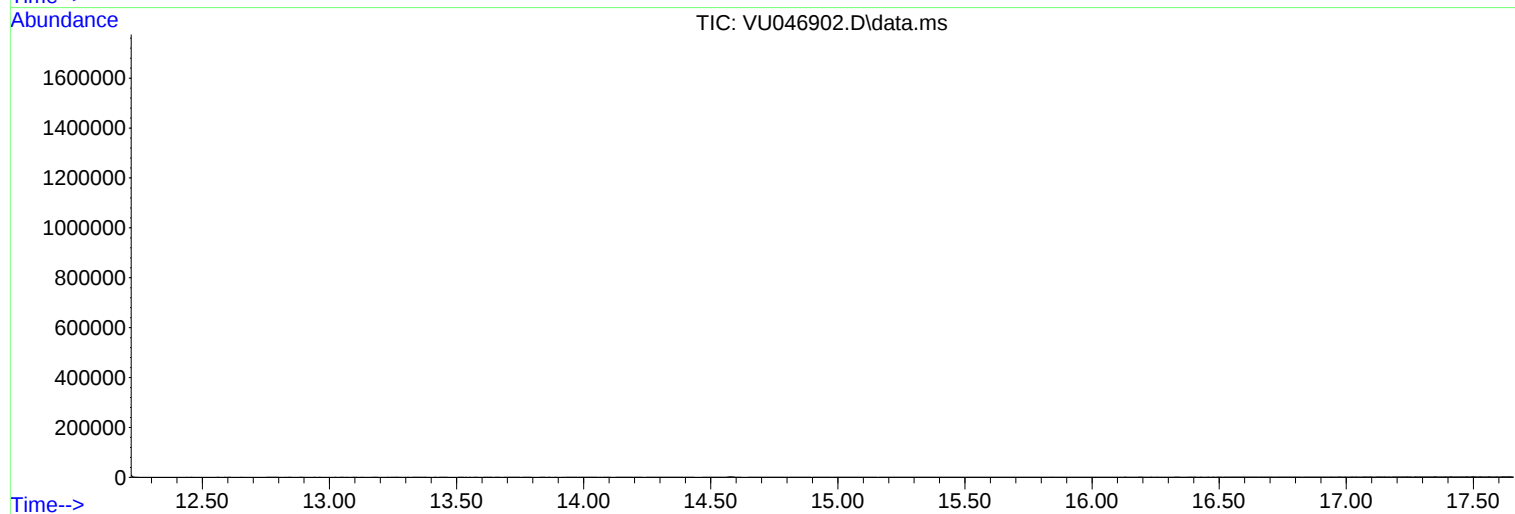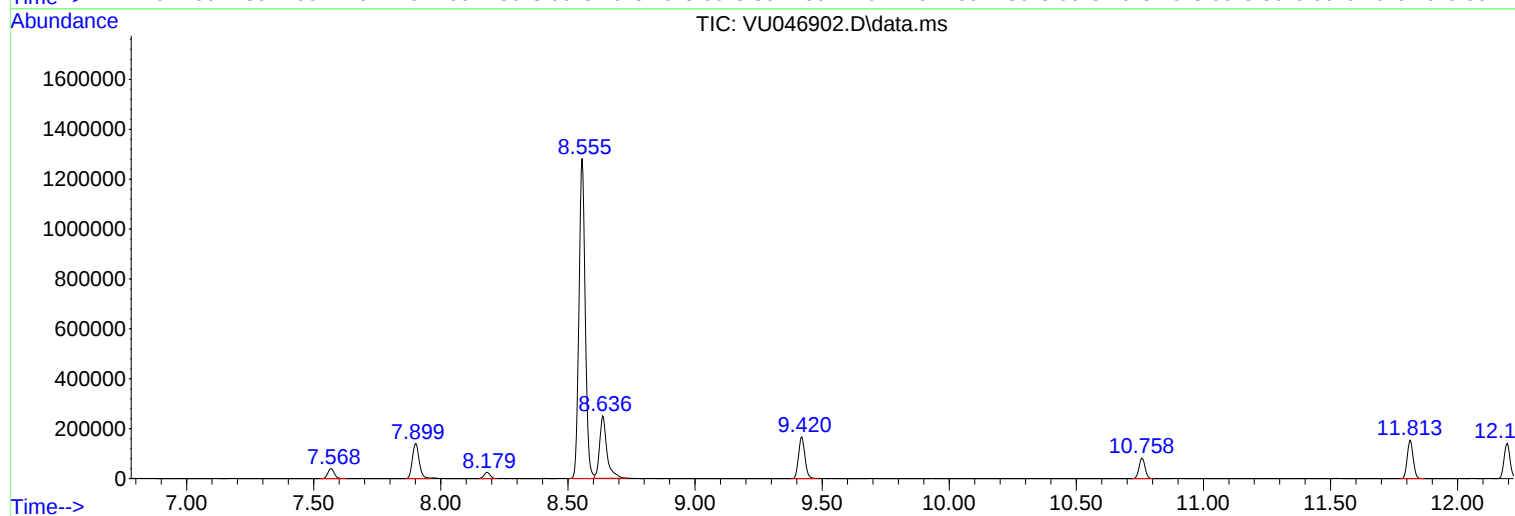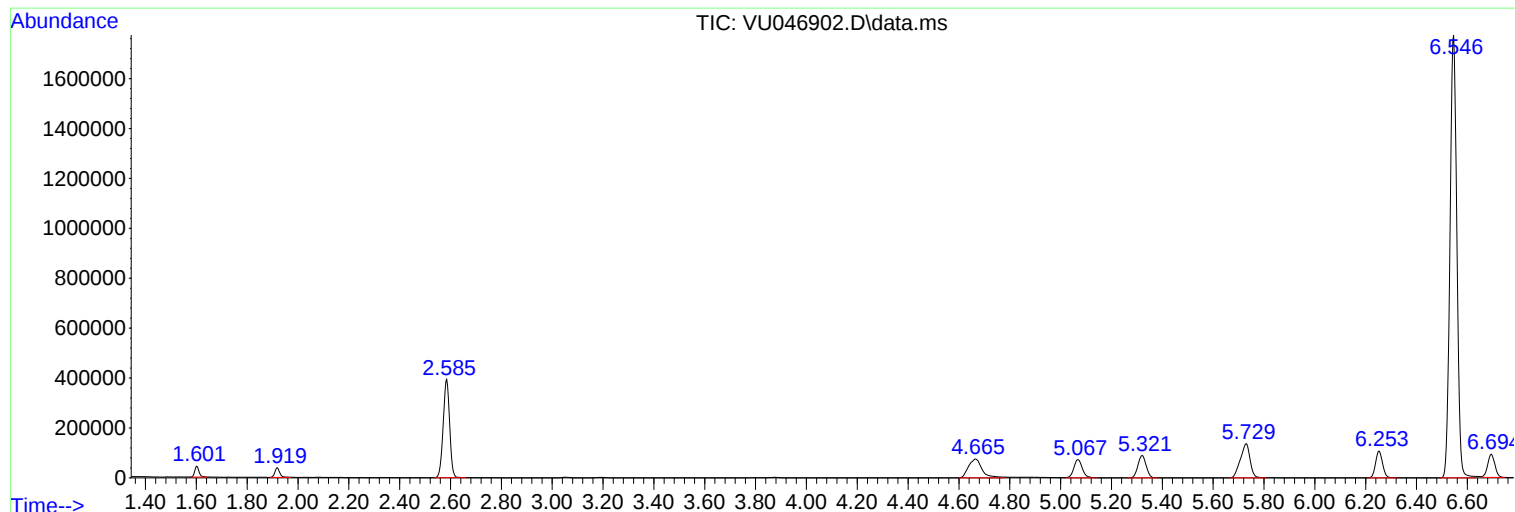

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046902.D
Acq On : 28 Jan 2022 19:02
Operator : SY/MD
Sample : N1273-16 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046902.D
Acq On : 28 Jan 2022 19:02
Operator : SY/MD
Sample : N1273-16 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
