

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
 Data File : VU046904.D
 Acq On : 28 Jan 2022 19:51
 Operator : SY/MD
 Sample : N1273-18 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHL6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rBV	43015	51116	5.15%	1.070%
2	1.919	171	180	194	rBV	36945	48774	4.92%	1.021%
3	2.578	372	385	402	rBV3	107271	210125	21.18%	4.399%
4	4.671	1012	1036	1066	rBV3	109454	362995	36.59%	7.600%
5	5.067	1144	1159	1179	rBV	72899	163657	16.50%	3.426%
6	5.321	1223	1238	1254	rBV2	13935	30529	3.08%	0.639%
7	5.729	1344	1365	1391	rBV2	137468	366565	36.95%	7.675%
8	6.253	1514	1528	1552	rBV	106734	207923	20.96%	4.353%
9	6.546	1605	1619	1640	rBV	225726	424864	42.82%	8.895%
10	6.694	1650	1665	1686	rVB	91400	179008	18.04%	3.748%
11	7.568	1926	1937	1955	rBV2	38005	67213	6.77%	1.407%
12	7.899	2026	2040	2061	rBV	137498	252956	25.50%	5.296%
13	8.182	2117	2128	2141	rBV	24851	40539	4.09%	0.849%
14	8.555	2230	2244	2259	rBV	563544	992115	100.00%	20.772%
15	8.639	2259	2270	2308	rVB	245369	485686	48.95%	10.169%
16	9.420	2499	2513	2533	rBV	167259	287779	29.01%	6.025%
17	10.758	2915	2929	2944	rBV	82819	132462	13.35%	2.773%
18	11.812	3243	3257	3276	rBV	154765	243612	24.55%	5.100%
19	12.195	3363	3376	3393	rVB	143782	228339	23.02%	4.781%




Sum of corrected areas: 4776257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046904.D
Acq On : 28 Jan 2022 19:51
Operator : SY/MD
Sample : N1273-18 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

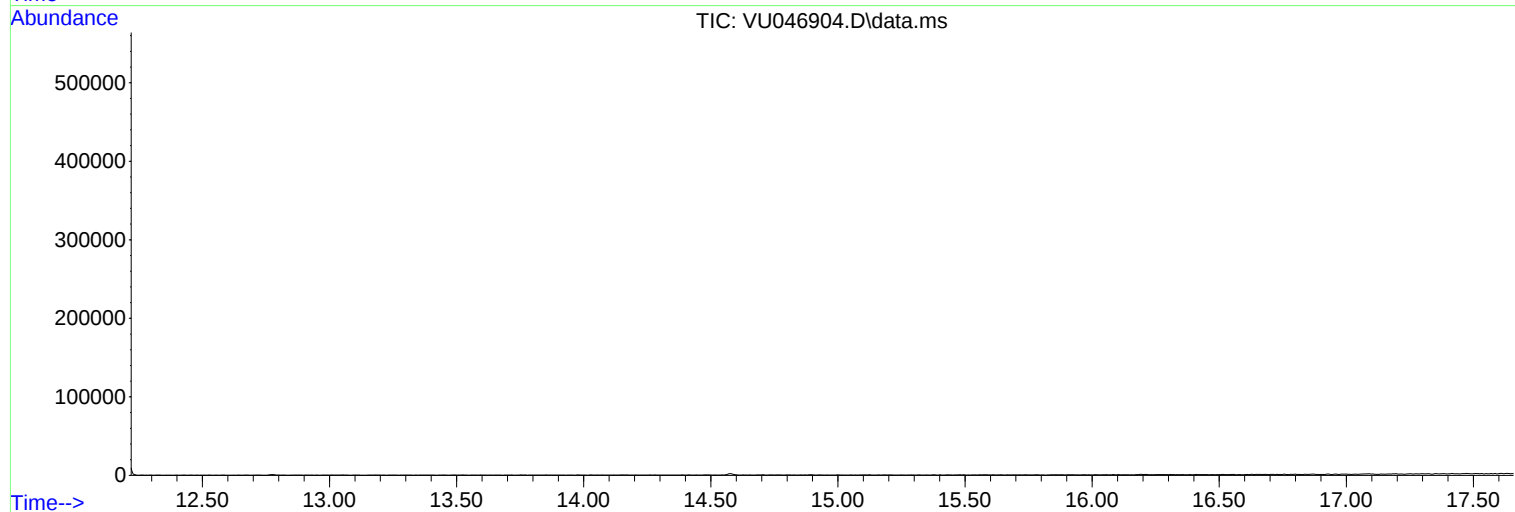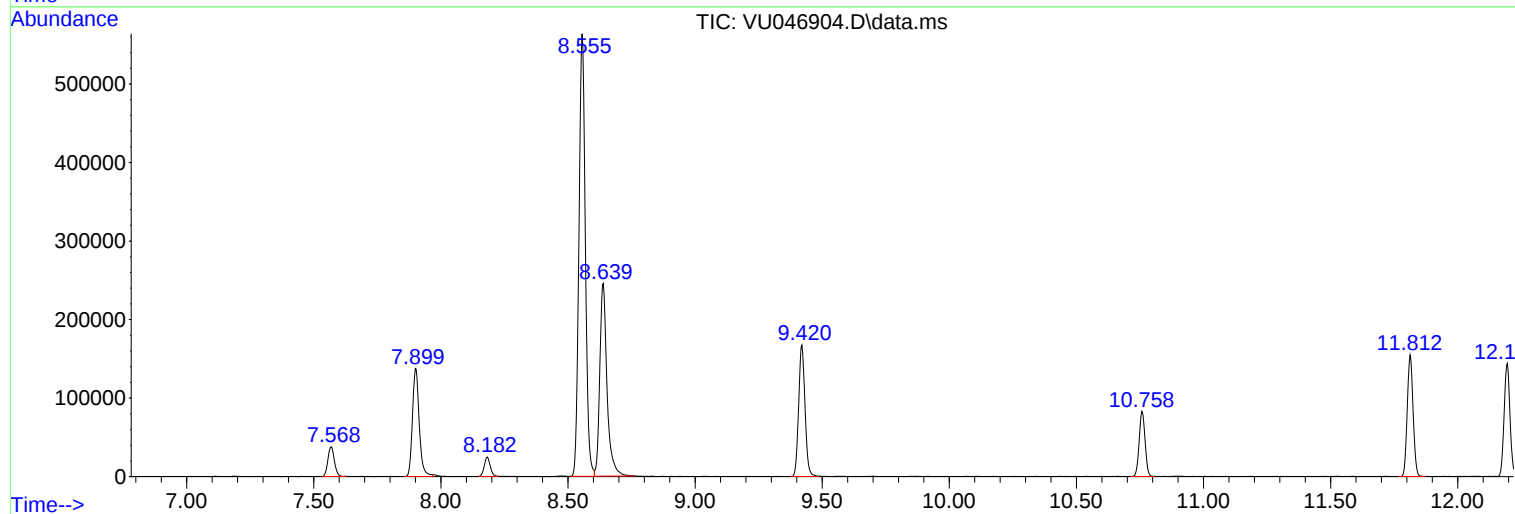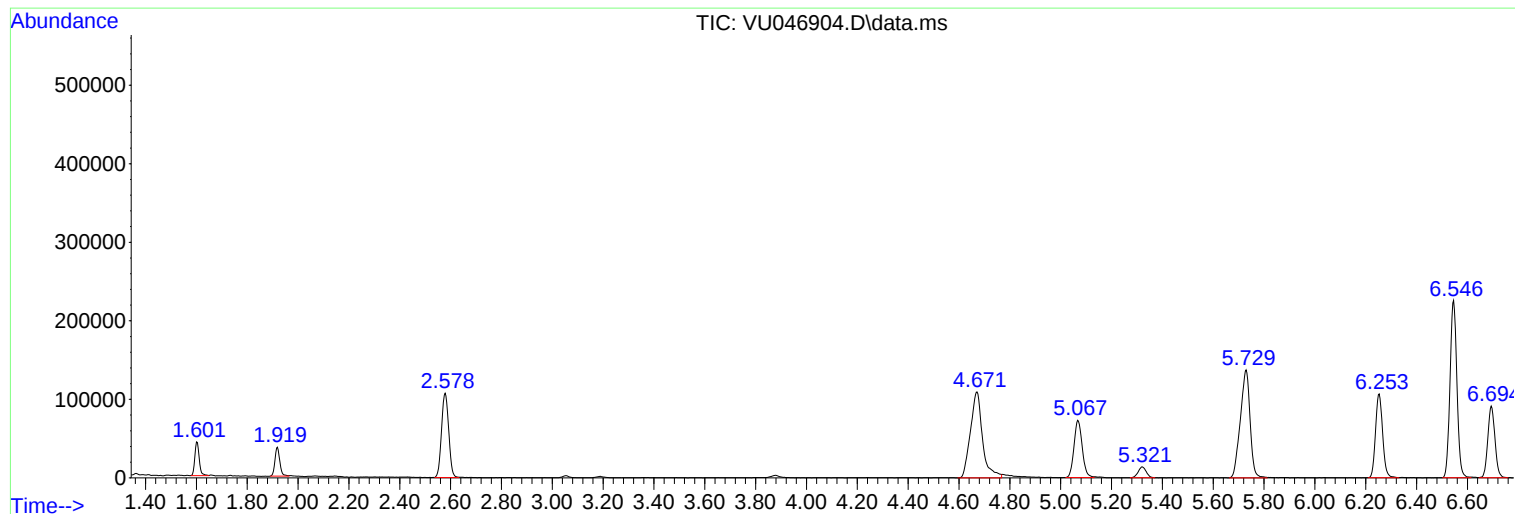

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046904.D
Acq On : 28 Jan 2022 19:51
Operator : SY/MD
Sample : N1273-18 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
Data File : VU046904.D
Acq On : 28 Jan 2022 19:51
Operator : SY/MD
Sample : N1273-18 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc