


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012822\
 Data File : VU046883.D
 Acq On : 28 Jan 2022 08:58
 Operator : SY/MD
 Sample : BFB049
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB049

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Feb 03 02:56:36 2022

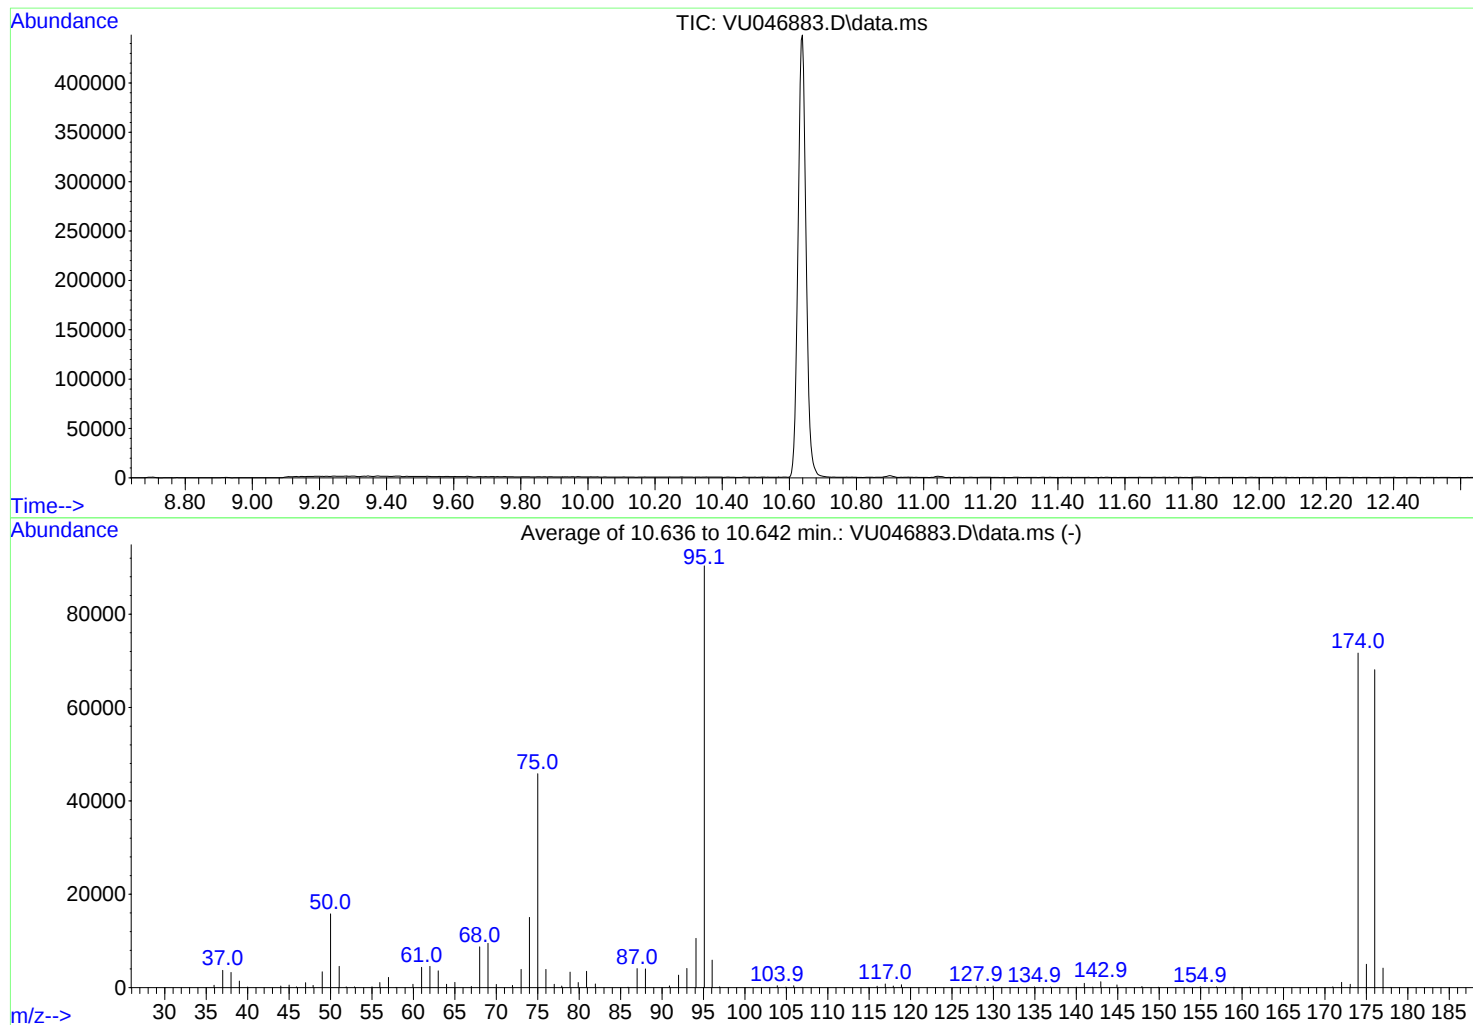

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	15804	PASS
75	95	30	80	50.7	45819	PASS
95	95	100	100	100.0	90349	PASS
96	95	5	9	6.5	5889	PASS
173	174	0.00	2	1.0	721	PASS
174	95	50	120	79.3	71677	PASS
175	174	5	9	7.0	4996	PASS
176	174	95	101	95.0	68096	PASS
177	176	5	9	6.1	4170	PASS

m/z	Abundance
35.90	419.0
38.00	106.0
44.00	250.0

Instrument :
MSVOA_U
ClientSampleId :
BFB049

m/z	Abundance
36.00	958.0
37.00	3720.0
38.00	3539.0
39.00	1572.0
40.00	155.0
44.00	636.0
45.00	616.0
45.90	186.0
47.00	1123.0
47.90	489.0
49.00	3531.0
50.00	16359.0
51.00	4664.0
51.90	183.0
52.90	159.0
55.00	187.0
56.00	1215.0
57.00	2306.0
60.00	757.0
61.00	4493.0
62.00	4645.0
63.00	3761.0
64.00	790.0
65.00	1176.0
67.00	194.0
68.00	9022.0
69.00	9575.0
70.00	711.0
71.90	486.0
73.00	4059.0
74.00	15341.0
75.00	47600.0
76.00	3968.0
77.00	663.0
77.90	319.0
78.90	3497.0
79.90	1112.0
80.90	3610.0
82.00	801.0
85.90	102.0
87.00	4099.0
88.00	4089.0
90.90	404.0
92.00	2666.0
93.00	4248.0
94.10	10567.0
95.10	92968.0
96.00	6139.0
97.00	144.0
103.90	437.0
104.90	179.0
105.90	419.0
106.90	102.0
114.90	145.0
115.90	329.0
117.00	817.0
117.90	418.0
118.90	645.0
127.90	458.0
129.00	198.0
130.00	363.0
135.00	154.0
136.90	137.0
141.00	971.0
141.90	116.0
142.90	1315.0
144.90	688.0
147.90	215.0
149.90	104.0
155.00	230.0
156.90	149.0
159.00	122.0
160.90	101.0
171.00	209.0
172.00	1223.0
173.00	676.0
174.00	72104.0
175.00	5099.0
176.00	67384.0
177.00	4261.0

Instrument :
MSVOA_U
ClientSampleId :
BFB049

m/z	Abundance
36.00	984.0
37.00	3847.0
38.00	3486.0
39.00	1440.0
40.00	142.0
44.00	594.0
45.00	577.0
45.90	198.0
47.00	1095.0
47.90	501.0
49.00	3499.0
50.00	16313.0
51.00	4667.0
51.90	181.0
52.90	184.0
55.00	192.0
56.00	1130.0
57.00	2236.0
57.90	113.0
60.00	756.0
61.00	4498.0
62.00	4684.0
63.00	3678.0
64.00	716.0
65.00	1171.0
67.00	237.0
68.00	9031.0
69.00	9843.0
70.00	697.0
71.90	503.0
73.00	4011.0
74.00	15493.0
75.00	47224.0
76.00	4053.0
77.00	785.0
77.90	357.0
78.90	3440.0
79.90	1109.0
80.90	3644.0
81.90	802.0
85.90	115.0
87.00	4194.0
88.00	4120.0
90.90	368.0
92.00	2780.0
93.00	4216.0
94.10	10919.0
95.10	93128.0
96.10	5976.0
97.00	171.0
103.90	440.0
105.00	154.0
105.90	434.0
106.90	100.0
114.90	110.0
116.00	321.0
116.90	820.0
117.90	369.0
118.90	651.0
127.90	393.0
129.00	194.0
130.00	343.0
134.90	184.0
136.90	153.0
140.00	133.0
141.00	969.0
141.90	118.0
142.90	1285.0
144.90	567.0
147.90	246.0
149.90	110.0
155.00	215.0
156.90	161.0
159.00	122.0
160.90	129.0
170.90	156.0
172.00	1146.0
173.10	733.0
174.00	73824.0
175.00	5111.0
176.00	70376.0
177.00	4235.0
177.90	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB049

m/z	Abundance
36.00	904.0
37.00	3568.0
38.00	3019.0
39.00	1242.0
40.00	130.0
44.00	518.0
45.00	497.0
45.90	147.0
47.00	975.0
47.90	464.0
49.00	3124.0
50.00	14739.0
51.10	4331.0
51.90	159.0
52.90	176.0
55.00	191.0
55.90	985.0
57.00	2018.0
57.90	129.0
59.90	693.0
61.00	4078.0
62.00	4334.0
63.00	3363.0
64.00	640.0
65.00	1048.0
67.00	253.0
68.00	8191.0
69.00	9050.0
70.00	610.0
72.00	501.0
73.00	3663.0
74.00	14318.0
75.00	42632.0
76.00	3742.0
77.00	736.0
77.90	369.0
78.90	3075.0
79.90	1044.0
80.90	3249.0
81.90	767.0
85.90	111.0
87.00	3943.0
88.00	3821.0
90.90	326.0
92.00	2621.0
93.00	3902.0
94.10	10187.0
95.10	84952.0
96.10	5552.0
96.90	177.0
103.90	415.0
105.00	129.0
105.90	410.0
115.90	301.0
116.90	705.0
117.90	281.0
118.90	588.0
127.90	301.0
128.90	163.0
129.90	303.0
131.00	125.0
134.90	169.0
136.90	164.0
140.00	136.0
140.90	888.0
142.00	131.0
143.00	1202.0
144.90	468.0
147.90	214.0
149.90	111.0
154.90	215.0
156.90	158.0
159.00	105.0
160.90	123.0
170.90	118.0
172.00	985.0
173.10	753.0
174.00	69104.0
175.00	4778.0
176.00	66528.0
177.00	4015.0
178.00	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB049