

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
 Data File : VU046936.D
 Acq On : 31 Jan 2022 23:10
 Operator : SY/MD
 Sample : N1328-07DL 500X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HM6DL

Quant Time: Feb 01 03:01:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 01 01:39:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	101495	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	116723	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	46920	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	53397	6.209	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	124.200%
7) Chloroethane-d5	1.919	69	39707	5.860	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	117.200%
11) 1,1-Dichloroethene-d2	2.575	65	20560	6.010	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	120.200%
20) 2-Butanone-d5	4.649	46	108586	42.619	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.240%
24) Chloroform-d	5.067	84	78532	5.202	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.000%
26) 1,2-Dichloroethane-d4	5.707	65	43730	5.319	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.400%
32) Benzene-d6	5.732	84	156179	4.553	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.000%
36) 1,2-Dichloropropane-d6	6.694	67	49469	4.803	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	7.903	98	119587	3.809	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.200%
43) trans-1,3-Dichloroprop...	8.182	79	18003	3.980	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.600%
46) 2-Hexanone-d5	8.636	63	106216	39.657	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.320%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	45618	4.411	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.200%
66) 1,2-Dichlorobenzene-d4	12.195	152	40759	4.632	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.600%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	8.555	164	29805	5.136	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046936.D
Acq On : 31 Jan 2022 23:10
Operator : SY/MD
Sample : N1328-07DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HM6DL


Quant Time: Feb 01 03:01:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 01 01:39:38 2022
Response via : Initial Calibration

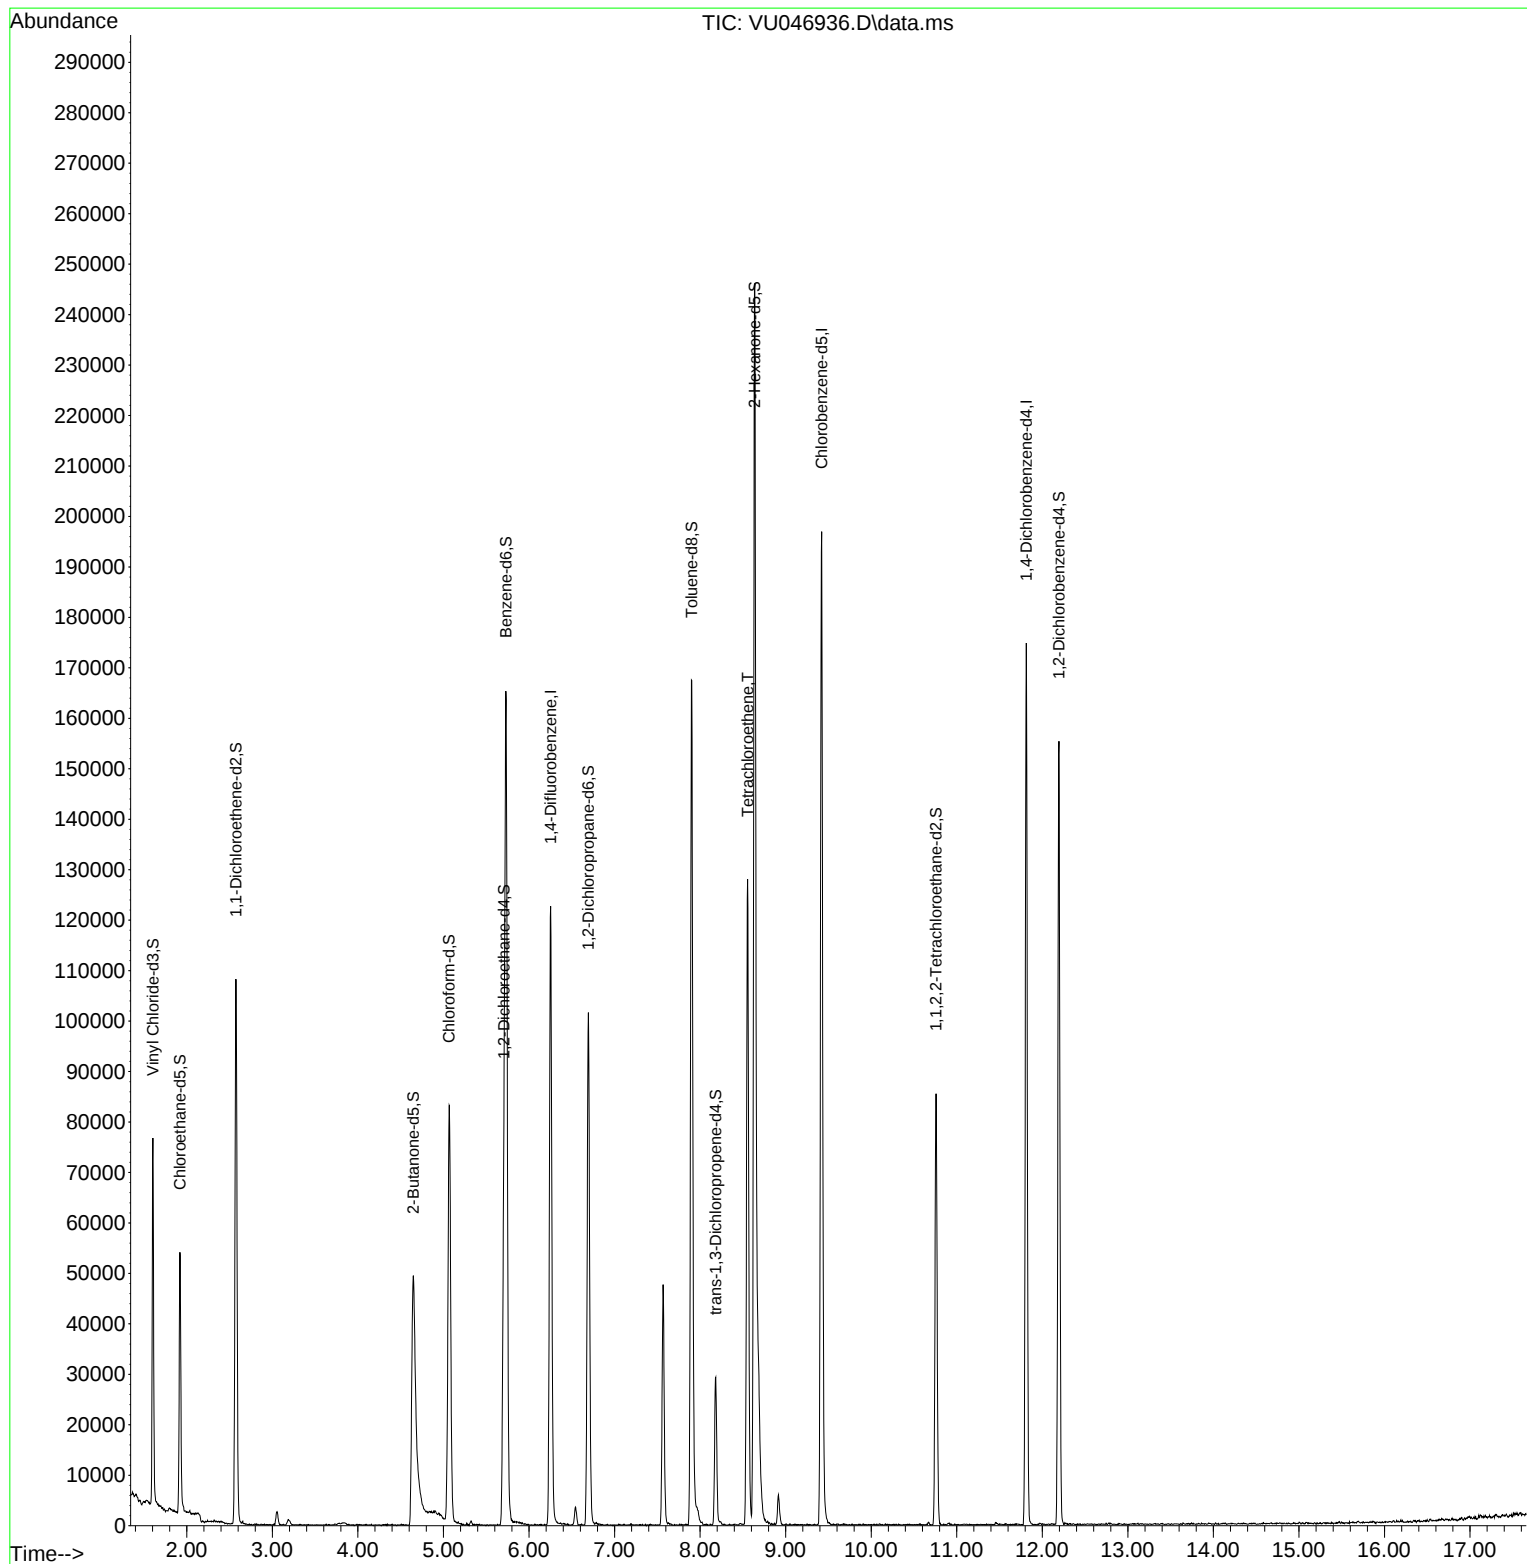

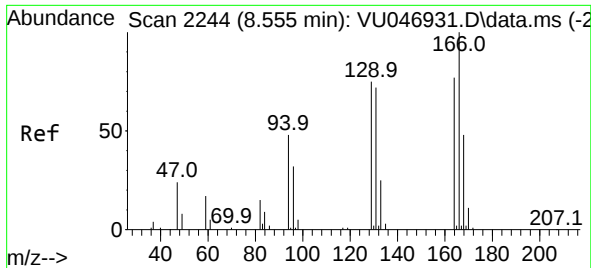

#47
Tetrachloroethene
Concen: 5.136 ug/L
RT: 8.555 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU046936.D
Acq: 31 Jan 2022 23:10

Instrument :
MSVOA_U
ClientSampleId :
C0HM6DL

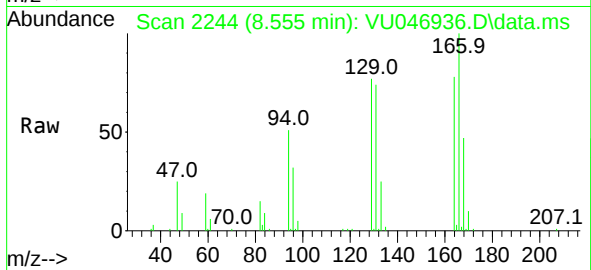

Tgt Ion:	164	Resp:	29805
Ion	Ratio	Lower	Upper
164	100		
129	98.6	71.8	133.4
131	94.4	68.5	127.3
166	127.5	94.1	174.8

