

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
 Data File : VU046921.D
 Acq On : 31 Jan 2022 16:39
 Operator : SY/MD
 Sample : N1328-15 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HN4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	94	rVB	67149	76901	9.34%	1.705%
2	1.919	172	180	193	rBV	47771	63406	7.70%	1.406%
3	2.575	372	384	407	rBV3	109110	192796	23.41%	4.274%
4	4.668	1015	1035	1070	rBV3	88068	303376	36.83%	6.726%
5	5.067	1144	1159	1189	rBV	76749	174038	21.13%	3.859%
6	5.324	1224	1239	1251	rBV4	7354	17008	2.07%	0.377%
7	5.729	1344	1365	1386	rBV2	152220	400863	48.67%	8.887%
8	6.253	1511	1528	1549	rBV	118234	231972	28.16%	5.143%
9	6.546	1606	1619	1635	rBV	92834	170345	20.68%	3.777%
10	6.694	1649	1665	1690	rBV2	93882	184937	22.45%	4.100%
11	7.568	1925	1937	1960	rVB2	44635	80205	9.74%	1.778%
12	7.903	2027	2041	2060	rBV	153645	289950	35.20%	6.428%
13	8.182	2115	2128	2144	rBV2	28388	48236	5.86%	1.069%
14	8.555	2231	2244	2259	rBV	470418	823622	100.00%	18.260%
15	8.639	2259	2270	2300	rVB	240059	483338	58.68%	10.716%
16	9.420	2499	2513	2535	rBV	187586	329058	39.95%	7.295%
17	10.758	2914	2929	2944	rVB	81294	131881	16.01%	2.924%
18	11.812	3246	3257	3274	rBV	170442	272569	33.09%	6.043%
19	12.195	3363	3376	3389	rBV	144549	236007	28.65%	5.232%




Sum of corrected areas: 4510508

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046921.D
Acq On : 31 Jan 2022 16:39
Operator : SY/MD
Sample : N1328-15 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

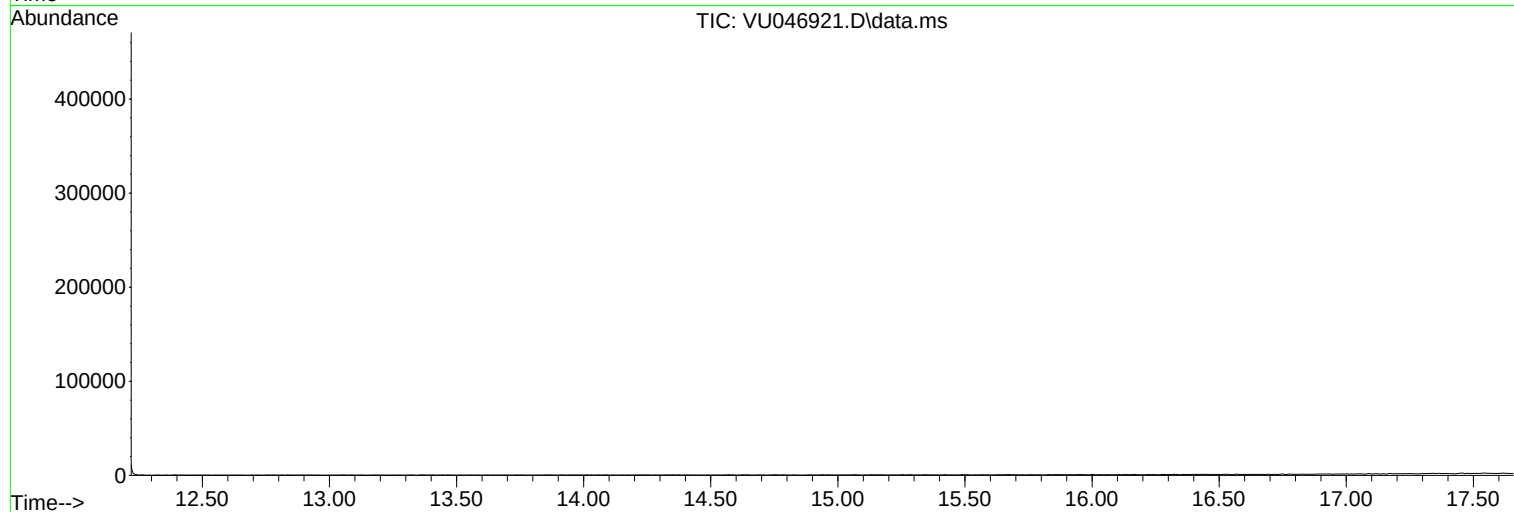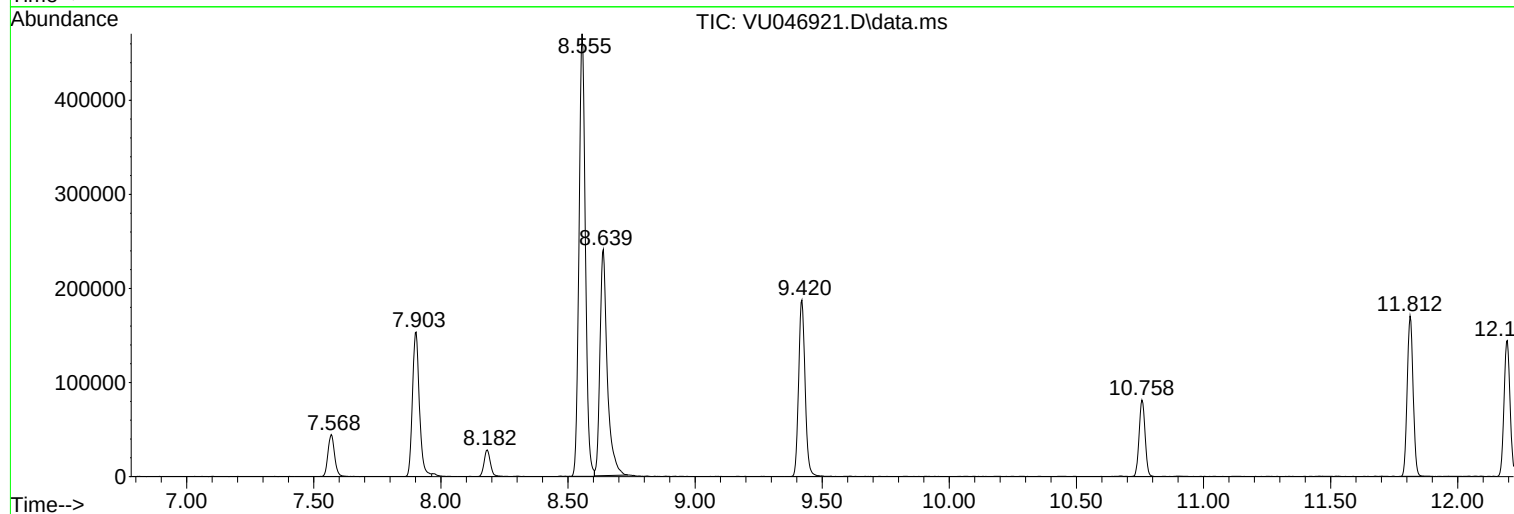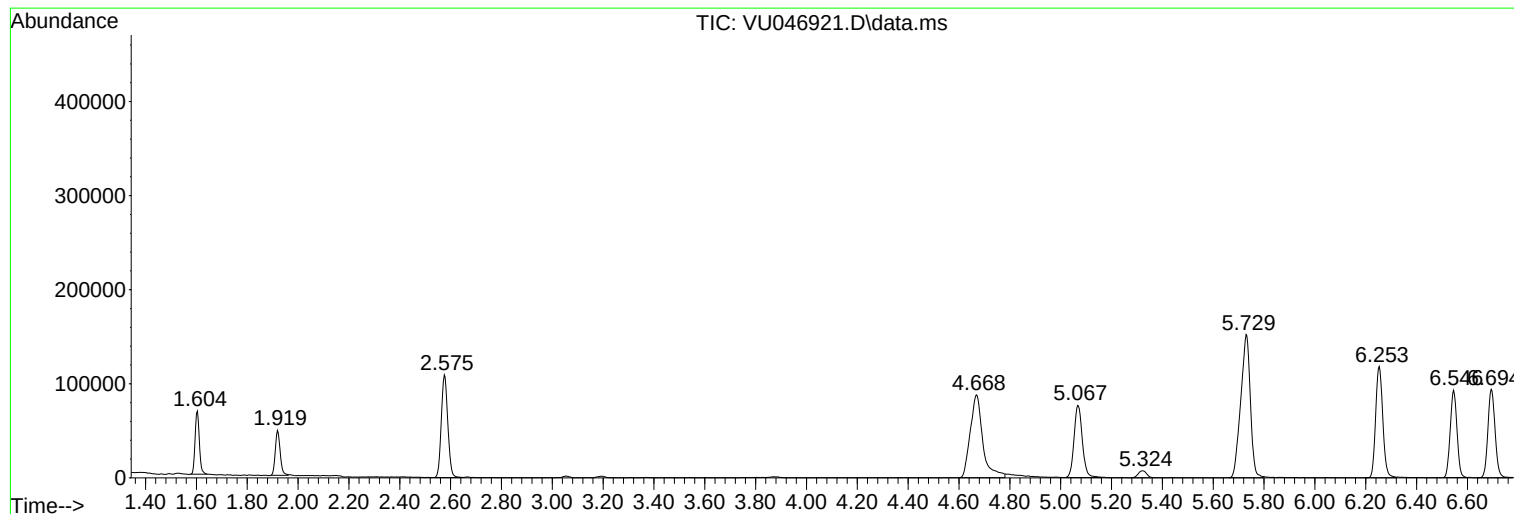

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046921.D
Acq On : 31 Jan 2022 16:39
Operator : SY/MD
Sample : N1328-15 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046921.D
Acq On : 31 Jan 2022 16:39
Operator : SY/MD
Sample : N1328-15 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc