

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
 Data File : VU046927.D
 Acq On : 31 Jan 2022 19:06
 Operator : SY/MD
 Sample : N1273-15 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHL3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU046927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	111	rVB	53628	82896	6.09%	1.491%
2	1.919	171	180	202	rBV	34255	62897	4.62%	1.131%
3	2.565	369	381	396	rVB3	118788	211454	15.54%	3.803%
4	3.874	775	788	805	rVB3	8169	18926	1.39%	0.340%
5	4.668	1016	1035	1077	rBV2	111551	359231	26.41%	6.461%
6	5.067	1143	1159	1182	rBV	80220	179190	13.17%	3.223%
7	5.726	1344	1364	1386	rBV2	161915	423404	31.12%	7.616%
8	6.250	1512	1527	1549	rBV	134002	259622	19.09%	4.670%
9	6.543	1605	1618	1633	rBV	152217	280898	20.65%	5.052%
10	6.694	1650	1665	1684	rVB	99649	193864	14.25%	3.487%
11	7.568	1924	1937	1958	rBV2	46868	84398	6.20%	1.518%
12	7.899	2026	2040	2058	rBV	174372	318072	23.38%	5.721%
13	8.182	2115	2128	2144	rBV2	27525	50986	3.75%	0.917%
14	8.555	2229	2244	2261	rBV	775749	1360338	100.00%	24.468%
15	8.658	2261	2276	2305	rVB	222229	537509	39.51%	9.668%
16	9.420	2500	2513	2537	rBV	201844	368076	27.06%	6.620%
17	10.764	2914	2931	2944	rVB	88197	144619	10.63%	2.601%
18	11.816	3246	3258	3277	rVB	210999	329451	24.22%	5.926%
19	12.063	3326	3335	3349	rBV2	9085	14858	1.09%	0.267%
20	12.195	3364	3376	3394	rVB	172745	279075	20.52%	5.020%




Sum of corrected areas: 5559764

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046927.D
Acq On : 31 Jan 2022 19:06
Operator : SY/MD
Sample : N1273-15 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

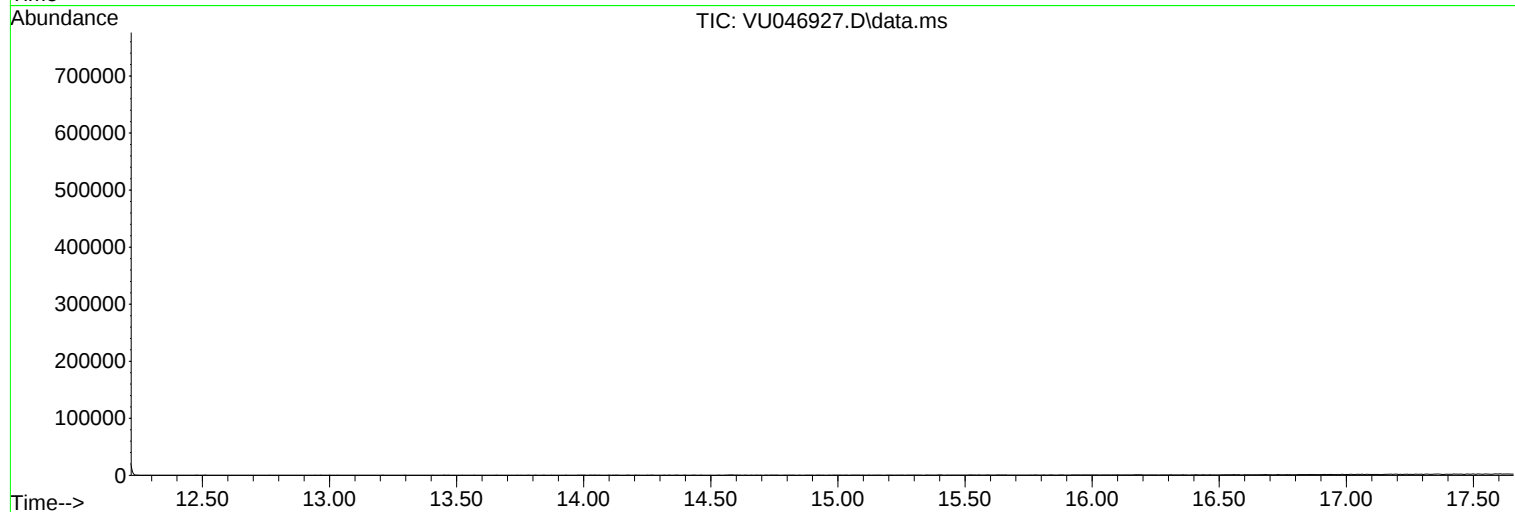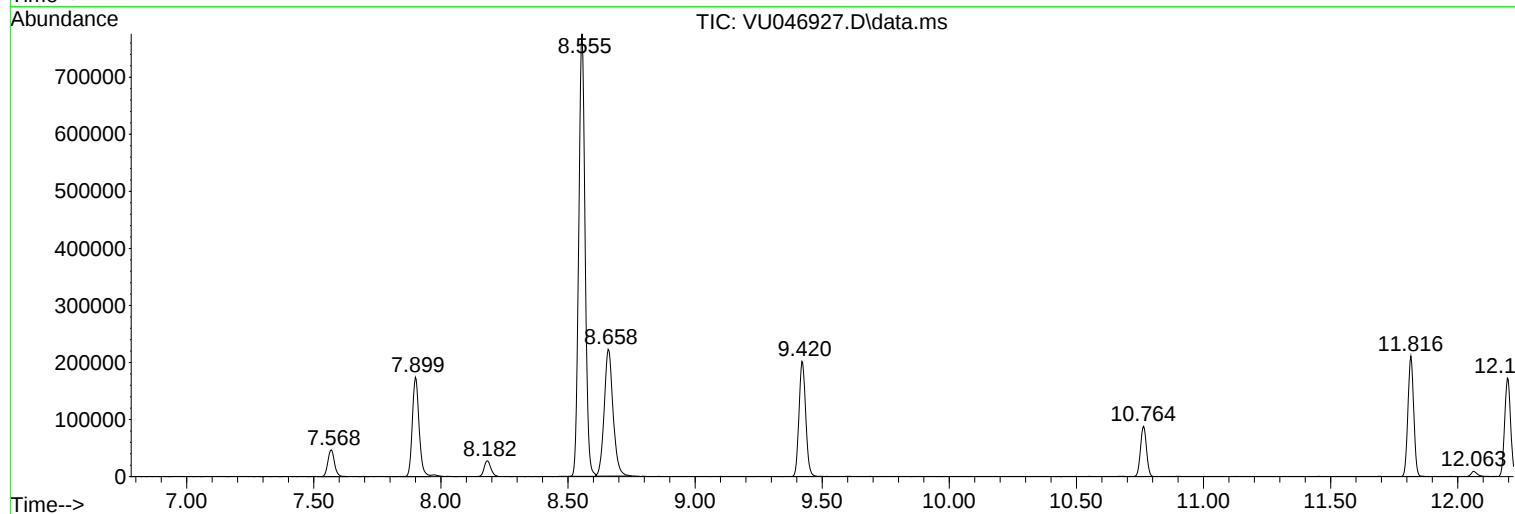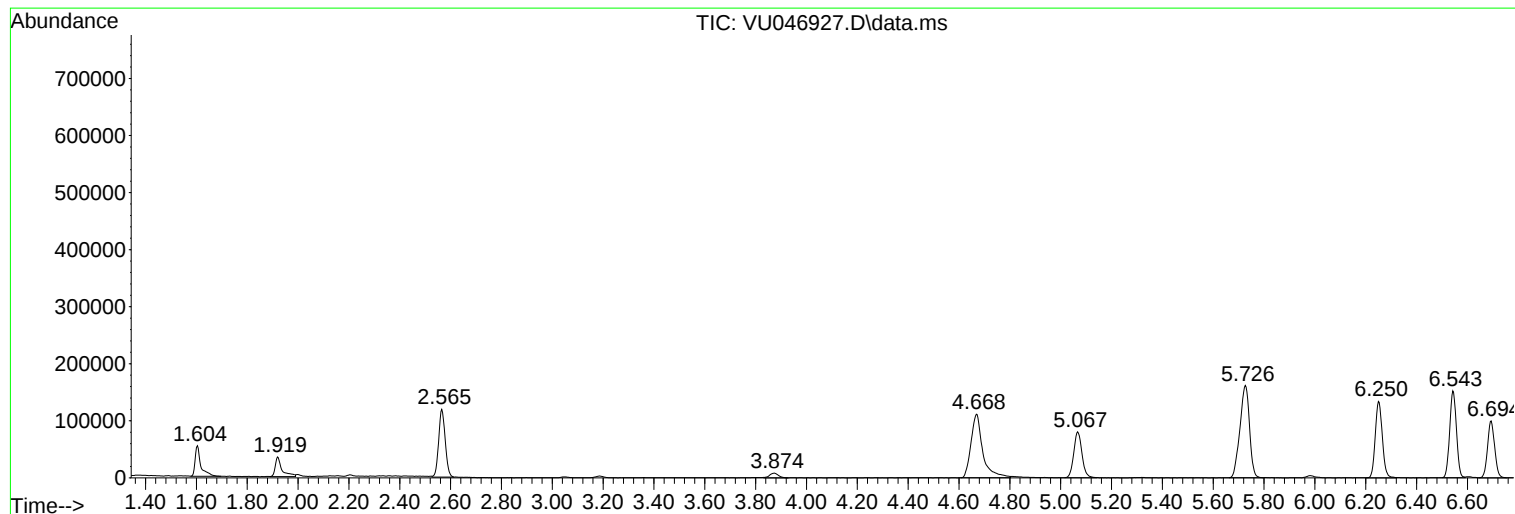

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046927.D
Acq On : 31 Jan 2022 19:06
Operator : SY/MD
Sample : N1273-15 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046927.D
Acq On : 31 Jan 2022 19:06
Operator : SY/MD
Sample : N1273-15 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc