

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
 Data File : VU046928.D
 Acq On : 31 Jan 2022 19:30
 Operator : SY/MD
 Sample : N1273-18 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHL6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	97	rBV	70767	91874	5.93%	1.420%
2	1.919	172	180	200	rBV	44907	67510	4.35%	1.043%
3	2.575	371	384	403	rVB3	180638	353472	22.80%	5.463%
4	3.189	559	575	588	rBV	7864	16861	1.09%	0.261%
5	4.668	1014	1035	1084	rBV3	157367	476366	30.72%	7.362%
6	5.067	1144	1159	1183	rVB2	82821	185183	11.94%	2.862%
7	5.317	1222	1237	1254	rBV	23229	51942	3.35%	0.803%
8	5.729	1343	1365	1387	rBV2	167442	435459	28.08%	6.730%
9	6.250	1513	1527	1550	rBV	126390	242902	15.67%	3.754%
10	6.542	1604	1618	1640	rBV	385383	726406	46.85%	11.227%
11	6.694	1652	1665	1686	rVB	103723	202000	13.03%	3.122%
12	7.568	1925	1937	1957	rBV2	48280	85212	5.50%	1.317%
13	7.899	2024	2040	2059	rBV	180039	324662	20.94%	5.018%
14	8.182	2116	2128	2140	rBV	31122	52717	3.40%	0.815%
15	8.555	2230	2244	2260	rBV	907338	1550564	100.00%	23.964%
16	8.645	2260	2272	2299	rVB	262974	552888	35.66%	8.545%
17	9.420	2500	2513	2532	rBV	198358	337477	21.76%	5.216%
18	10.761	2918	2930	2948	rBV	92455	147038	9.48%	2.273%
19	11.812	3246	3257	3277	rBV	187109	297042	19.16%	4.591%
20	12.195	3364	3376	3390	rBV	172401	272734	17.59%	4.215%




Sum of corrected areas: 6470309

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046928.D
Acq On : 31 Jan 2022 19:30
Operator : SY/MD
Sample : N1273-18 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

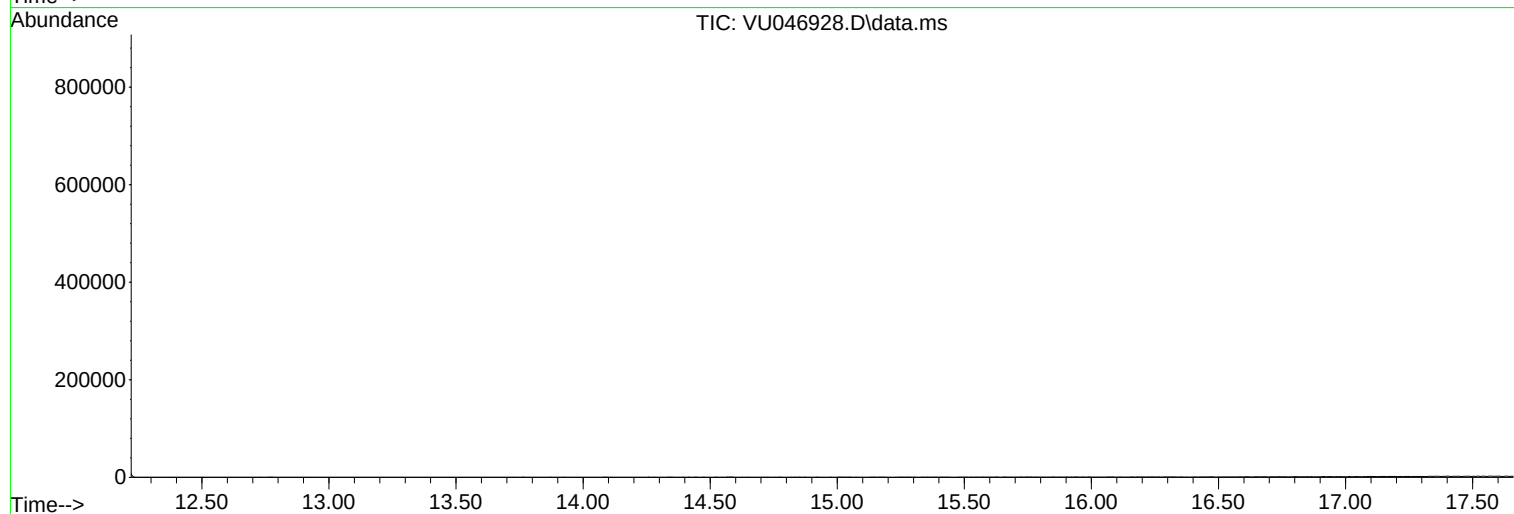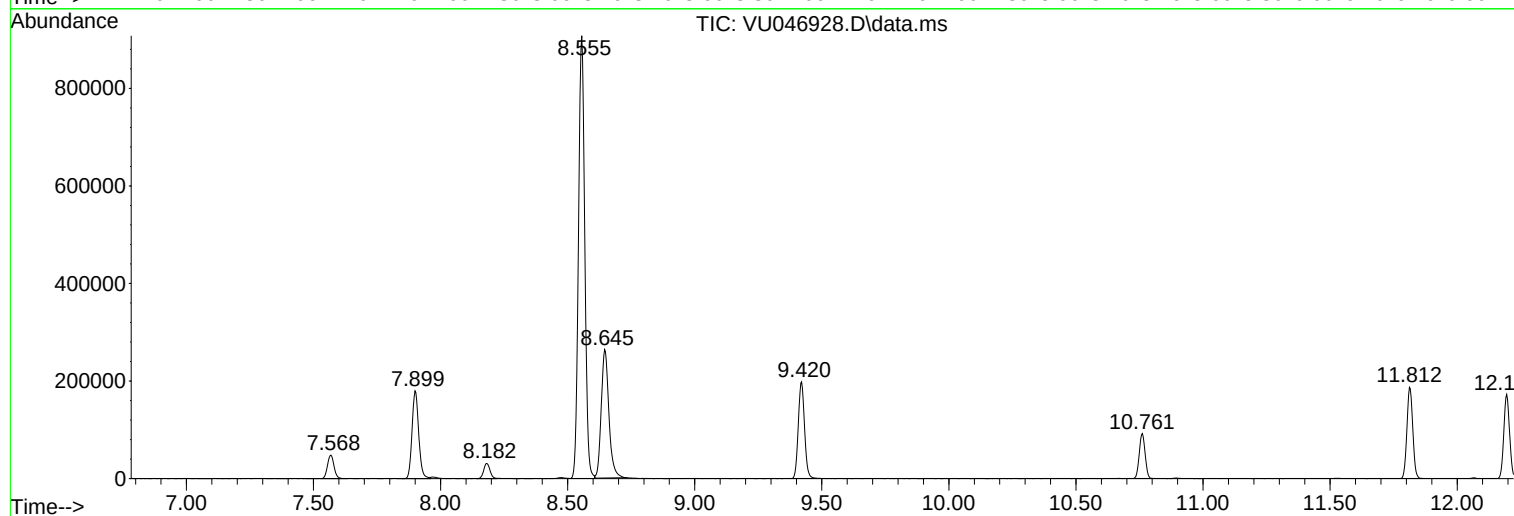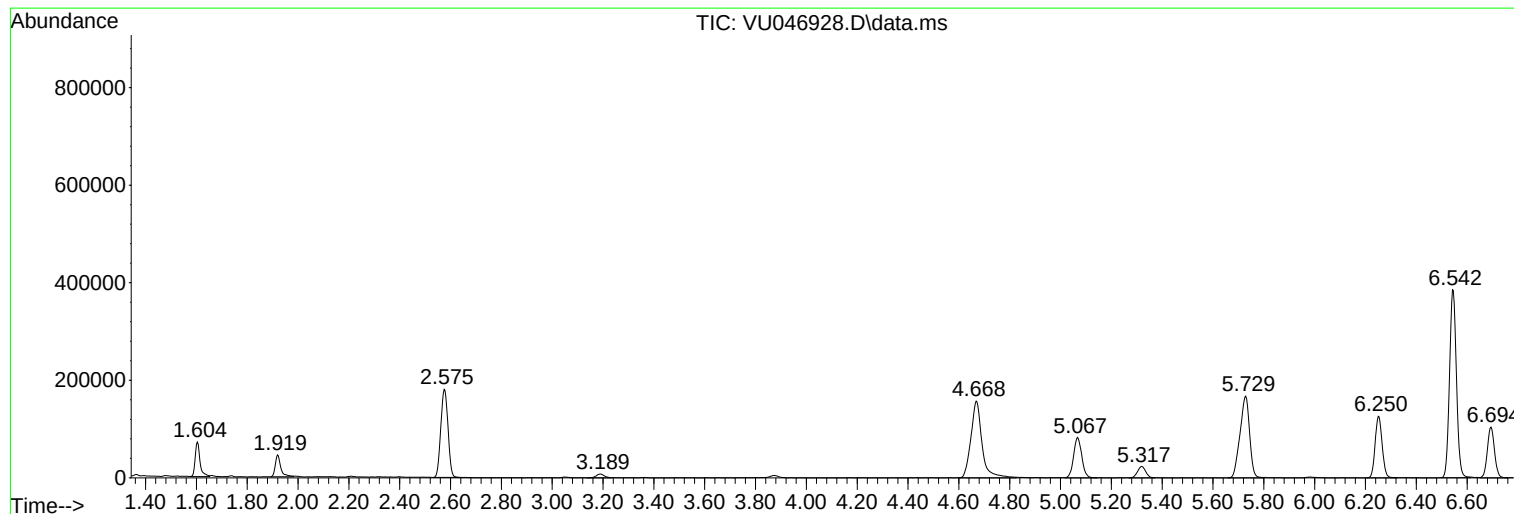

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046928.D
Acq On : 31 Jan 2022 19:30
Operator : SY/MD
Sample : N1273-18 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046928.D
Acq On : 31 Jan 2022 19:30
Operator : SY/MD
Sample : N1273-18 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc