

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
 Data File : VU046929.D
 Acq On : 31 Jan 2022 19:55
 Operator : SY/MD
 Sample : N1273-20 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHL8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046929.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	94	rBV	69864	80476	3.53%	0.978%
2	1.919	172	180	198	rBV	51528	69518	3.05%	0.844%
3	2.585	372	387	407	rBV4	283049	534927	23.49%	6.498%
4	4.665	1013	1034	1065	rBV2	71167	265650	11.67%	3.227%
5	5.067	1143	1159	1181	rVB	82084	182420	8.01%	2.216%
6	5.321	1222	1238	1260	rVB2	61081	141068	6.20%	1.714%
7	5.729	1344	1365	1385	rBV2	167307	429255	18.85%	5.214%
8	6.253	1513	1528	1551	rBV	126102	241735	10.62%	2.936%
9	6.546	1603	1619	1648	rBV	1218526	2277064	100.00%	27.660%
10	6.694	1652	1665	1683	rVB2	103761	207353	9.11%	2.519%
11	7.568	1925	1937	1954	rBV	48956	85465	3.75%	1.038%
12	7.899	2022	2040	2059	rBV	174297	324902	14.27%	3.947%
13	8.182	2117	2128	2142	rBV	29466	50979	2.24%	0.619%
14	8.555	2229	2244	2259	rBV	1010043	1753013	76.99%	21.294%
15	8.636	2259	2269	2309	rVB	261536	548596	24.09%	6.664%
16	9.420	2500	2513	2541	rVB	198813	346063	15.20%	4.204%
17	10.758	2917	2929	2946	rBV	86711	141718	6.22%	1.721%
18	11.812	3245	3257	3276	rBV	183497	291038	12.78%	3.535%
19	12.195	3363	3376	3394	rBV	156643	261173	11.47%	3.172%




Sum of corrected areas: 8232413

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046929.D
Acq On : 31 Jan 2022 19:55
Operator : SY/MD
Sample : N1273-20 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

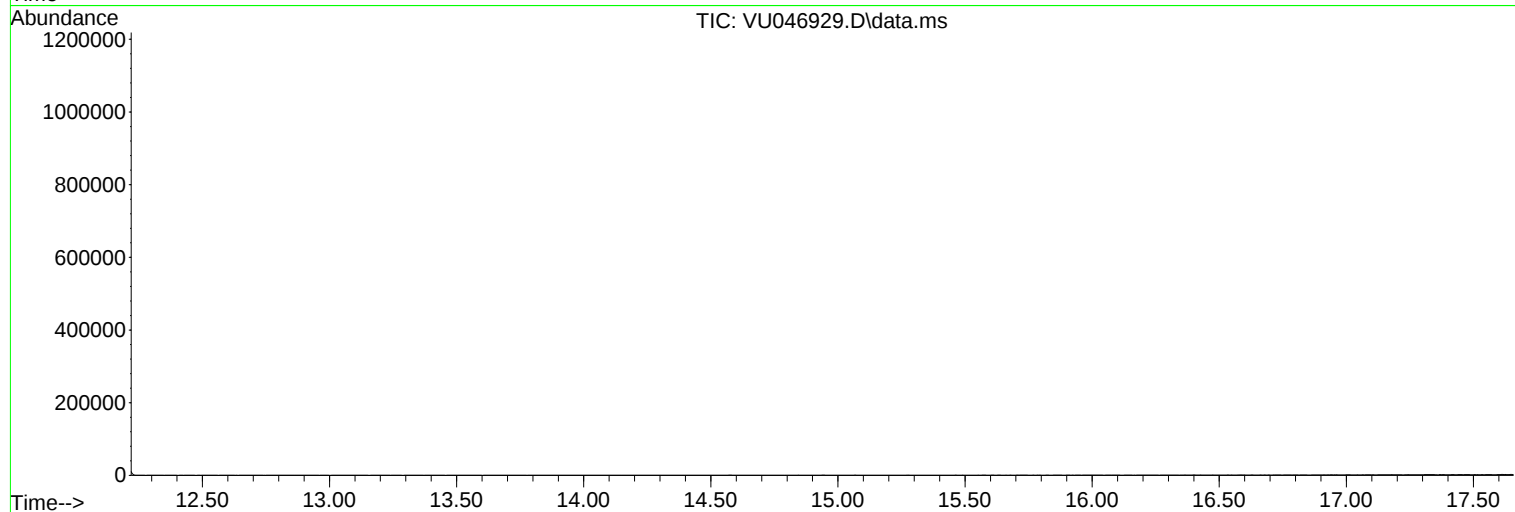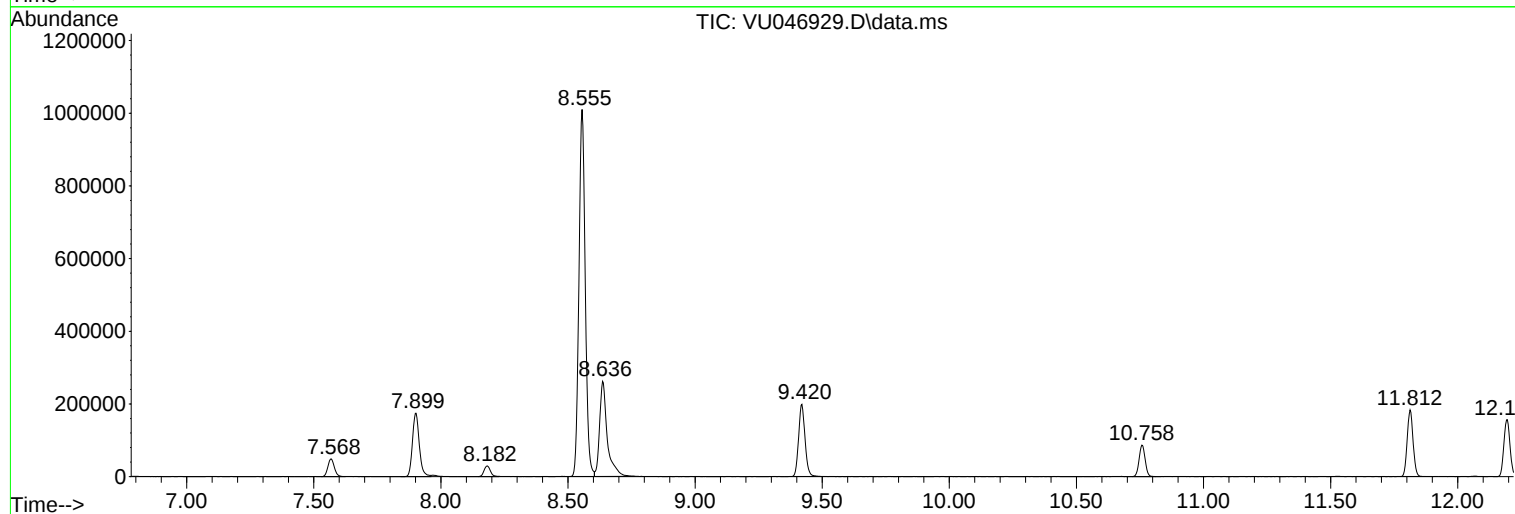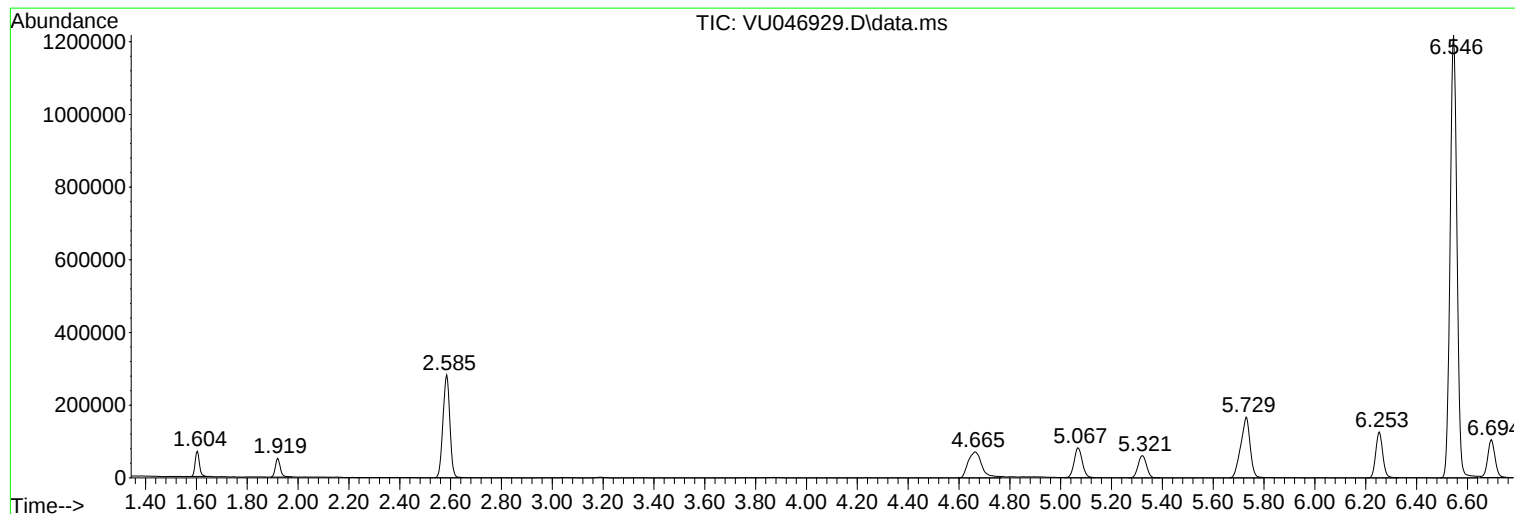

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046929.D
Acq On : 31 Jan 2022 19:55
Operator : SY/MD
Sample : N1273-20 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046929.D
Acq On : 31 Jan 2022 19:55
Operator : SY/MD
Sample : N1273-20 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
