

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
 Data File : VU046934.D
 Acq On : 31 Jan 2022 22:21
 Operator : SY/MD
 Sample : N1328-05DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HM4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046934.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	94	rBV	71295	82001	15.38%	2.153%
2	1.919	171	180	200	rBV	51515	70178	13.16%	1.843%
3	2.575	372	384	404	rBV	107181	174851	32.80%	4.591%
4	4.649	1014	1029	1068	rBV	51526	212824	39.92%	5.588%
5	5.070	1144	1160	1179	rBV2	80675	178926	33.57%	4.698%
6	5.729	1343	1365	1389	rBV2	164004	430789	80.81%	11.311%
7	6.253	1510	1528	1553	rBV	127176	245315	46.02%	6.441%
8	6.546	1609	1619	1629	rVB4	6561	10988	2.06%	0.289%
9	6.694	1652	1665	1686	rBV	101371	196944	36.95%	5.171%
10	7.568	1922	1937	1956	rBV	46939	82789	15.53%	2.174%
11	7.899	2028	2040	2059	rBV	167657	310986	58.34%	8.165%
12	8.182	2117	2128	2144	rBV2	29966	50859	9.54%	1.335%
13	8.555	2232	2244	2258	rBV	106435	184287	34.57%	4.839%
14	8.639	2258	2270	2313	rVB	259495	533072	100.00%	13.997%
15	8.915	2347	2356	2368	rVB2	5959	9218	1.73%	0.242%
16	9.420	2500	2513	2545	rBV	201613	347554	65.20%	9.126%
17	10.758	2916	2929	2947	rVB	87463	143797	26.98%	3.776%
18	11.812	3244	3257	3278	rVB	178901	287395	53.91%	7.546%
19	12.192	3364	3375	3392	rVB	158118	255792	47.98%	6.716%




Sum of corrected areas: 3808565

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046934.D
Acq On : 31 Jan 2022 22:21
Operator : SY/MD
Sample : N1328-05DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HM4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

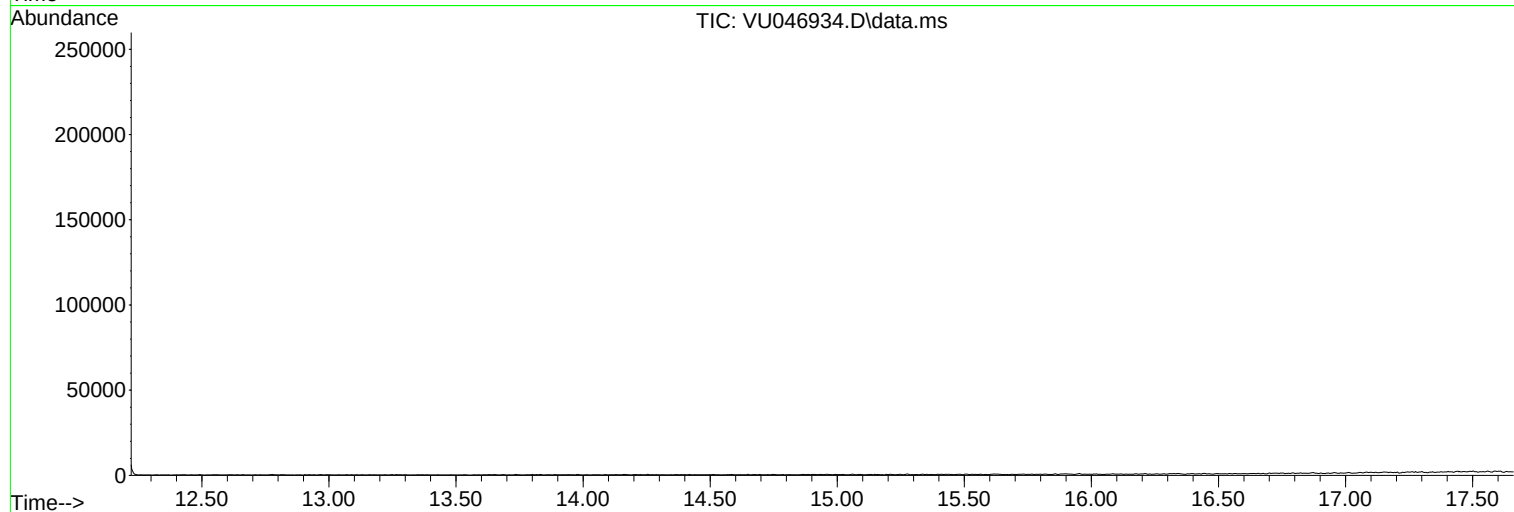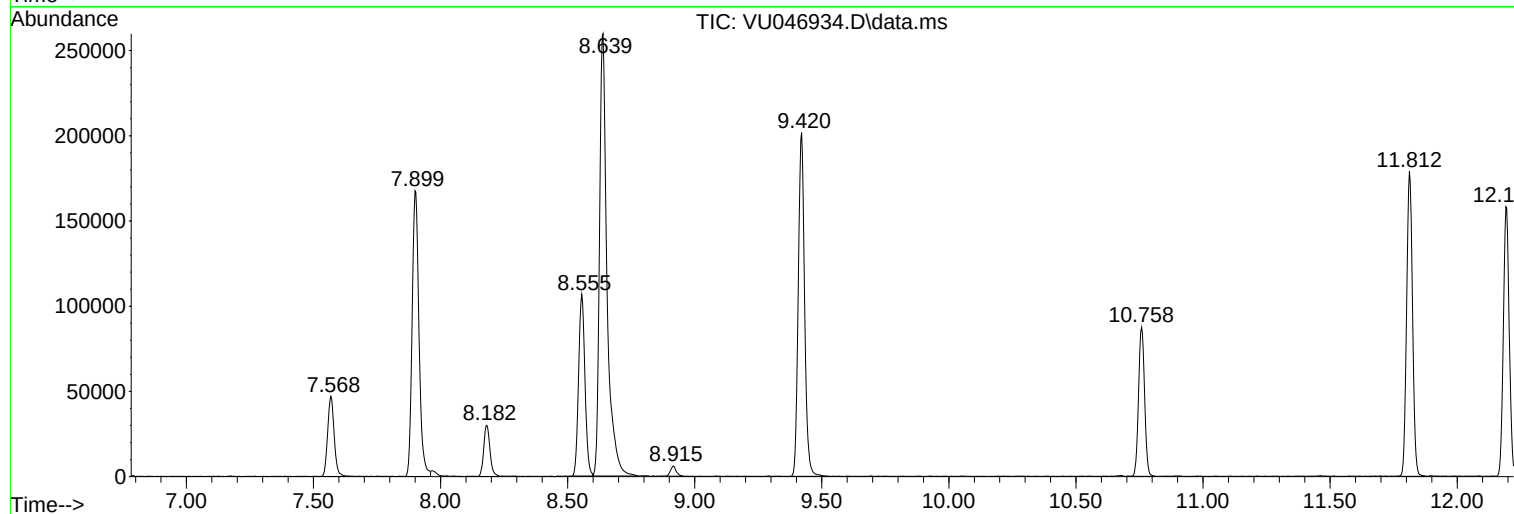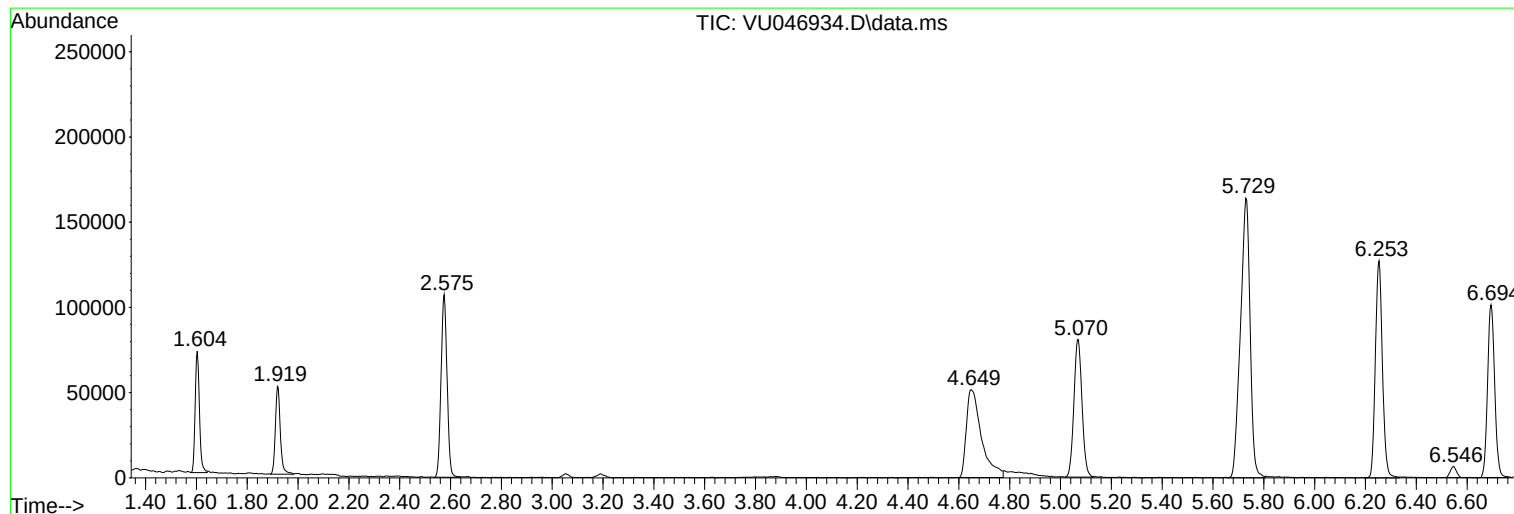

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046934.D
Acq On : 31 Jan 2022 22:21
Operator : SY/MD
Sample : N1328-05DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HM4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046934.D
Acq On : 31 Jan 2022 22:21
Operator : SY/MD
Sample : N1328-05DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HM4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc