

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
 Data File : VU046935.D
 Acq On : 31 Jan 2022 22:46
 Operator : SY/MD
 Sample : N1328-06DL 500X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HM5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046935.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	103	rVB	75504	86921	16.08%	2.243%
2	1.919	171	180	196	rBV	51822	70151	12.98%	1.810%
3	2.575	371	384	397	rBV	111385	182022	33.67%	4.696%
4	4.649	1013	1029	1084	rBV	49159	196533	36.35%	5.071%
5	5.070	1144	1160	1182	rBV	83319	184317	34.09%	4.756%
6	5.729	1344	1365	1395	rBV2	166957	441389	81.65%	11.389%
7	6.253	1512	1528	1548	rBV	122542	235307	43.53%	6.071%
8	6.546	1611	1619	1628	rVB6	3765	6590	1.22%	0.170%
9	6.694	1649	1665	1687	rBV	102112	201780	37.32%	5.206%
10	7.568	1925	1937	1954	rBV2	47912	84052	15.55%	2.169%
11	7.903	2027	2041	2060	rBV	174209	320053	59.20%	8.258%
12	8.182	2117	2128	2140	rBV2	30581	52242	9.66%	1.348%
13	8.555	2232	2244	2258	rBV	135361	232154	42.94%	5.990%
14	8.636	2258	2269	2305	rVB	251843	540619	100.00%	13.949%
15	8.915	2347	2356	2368	rBV2	5388	9155	1.69%	0.236%
16	9.420	2499	2513	2535	rBV	195093	342209	63.30%	8.830%
17	10.758	2917	2929	2945	rBV	88416	147647	27.31%	3.810%
18	11.812	3246	3257	3276	rBV	177655	279524	51.70%	7.212%
19	12.195	3363	3376	3394	rVB	159719	263077	48.66%	6.788%




Sum of corrected areas: 3875742

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046935.D
Acq On : 31 Jan 2022 22:46
Operator : SY/MD
Sample : N1328-06DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HM5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

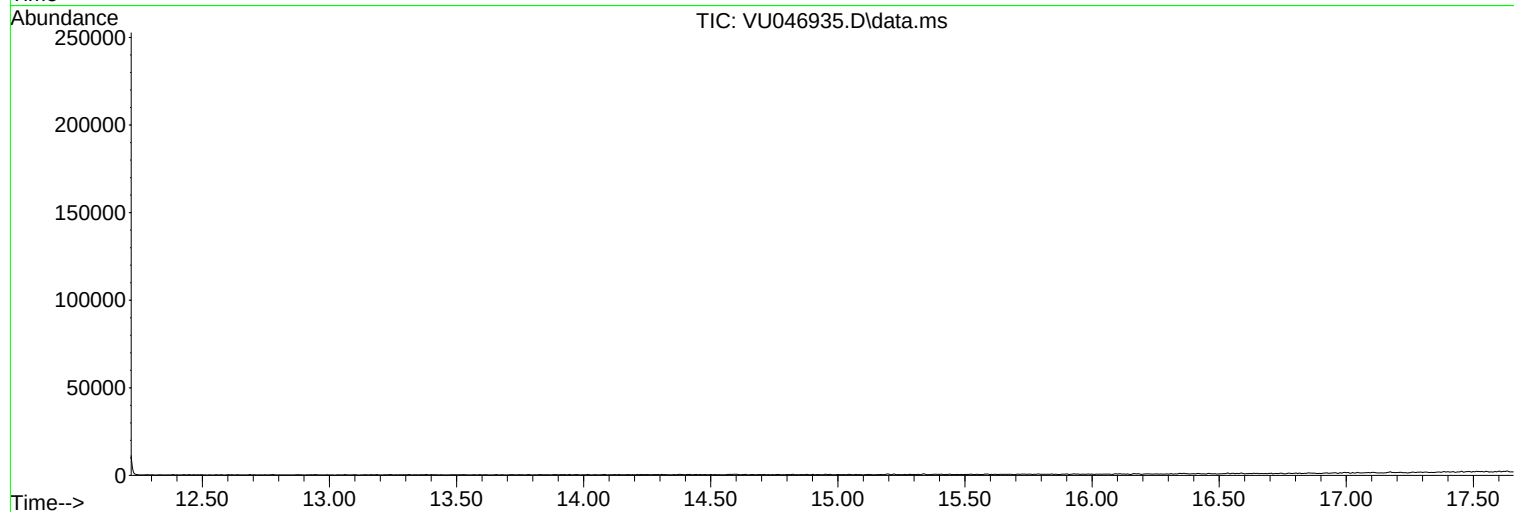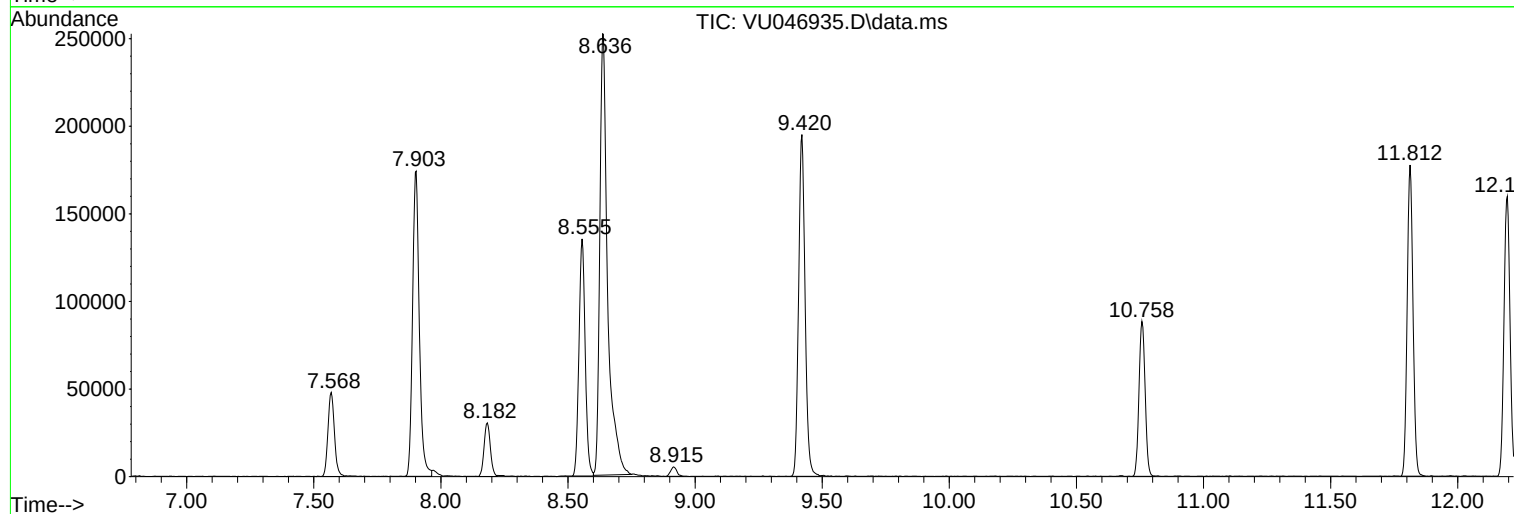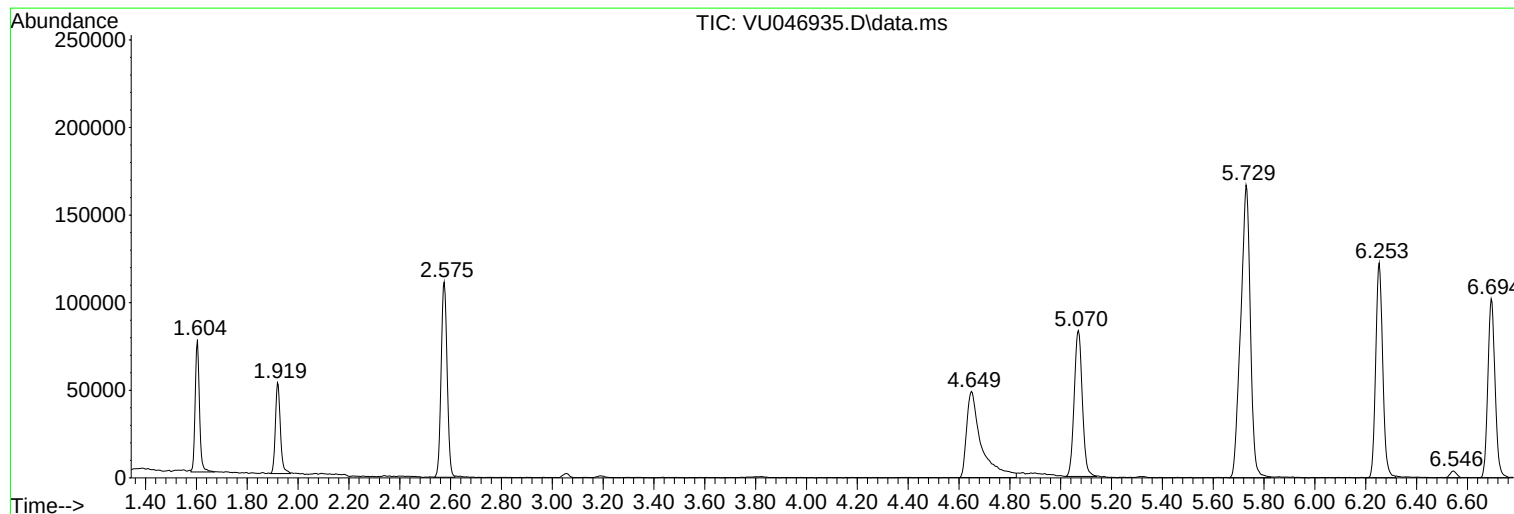

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046935.D
Acq On : 31 Jan 2022 22:46
Operator : SY/MD
Sample : N1328-06DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HM5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046935.D
Acq On : 31 Jan 2022 22:46
Operator : SY/MD
Sample : N1328-06DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HM5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc