

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
 Data File : VU046940.D
 Acq On : 01 Feb 2022 00:48
 Operator : SY/MD
 Sample : N1328-14DL 500X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HN3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	98	rVB	71573	80920	15.34%	2.152%
2	1.922	171	181	199	rBV	51631	70330	13.33%	1.871%
3	2.575	373	384	408	rBV	105321	173720	32.94%	4.621%
4	3.054	524	533	543	rBV3	4024	6807	1.29%	0.181%
5	4.649	1011	1029	1075	rBV2	44616	180245	34.17%	4.794%
6	5.070	1144	1160	1179	rVB	80128	178312	33.81%	4.743%
7	5.729	1344	1365	1389	rBV2	159225	423457	80.29%	11.264%
8	6.253	1513	1528	1555	rBV	121424	236625	44.86%	6.294%
9	6.546	1607	1619	1630	rBV3	11431	20702	3.93%	0.551%
10	6.694	1651	1665	1688	rBV	99200	194475	36.87%	5.173%
11	7.568	1925	1937	1951	rBV	45746	79334	15.04%	2.110%
12	7.903	2026	2041	2059	rBV	164835	306313	58.08%	8.148%
13	8.182	2118	2128	2142	rBV	29796	49713	9.43%	1.322%
14	8.555	2232	2244	2258	rBV2	116831	202635	38.42%	5.390%
15	8.639	2258	2270	2313	rVB	241502	527418	100.00%	14.029%
16	8.919	2348	2357	2371	rVB3	6010	10428	1.98%	0.277%
17	9.420	2500	2513	2541	rBV	195146	340479	64.56%	9.057%
18	10.758	2917	2929	2950	rVB	88061	145936	27.67%	3.882%
19	11.812	3245	3257	3274	rBV	175458	279142	52.93%	7.425%
20	12.192	3363	3375	3394	rBV	152531	252427	47.86%	6.715%




Sum of corrected areas: 3759418

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046940.D
Acq On : 01 Feb 2022 00:48
Operator : SY/MD
Sample : N1328-14DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HN3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

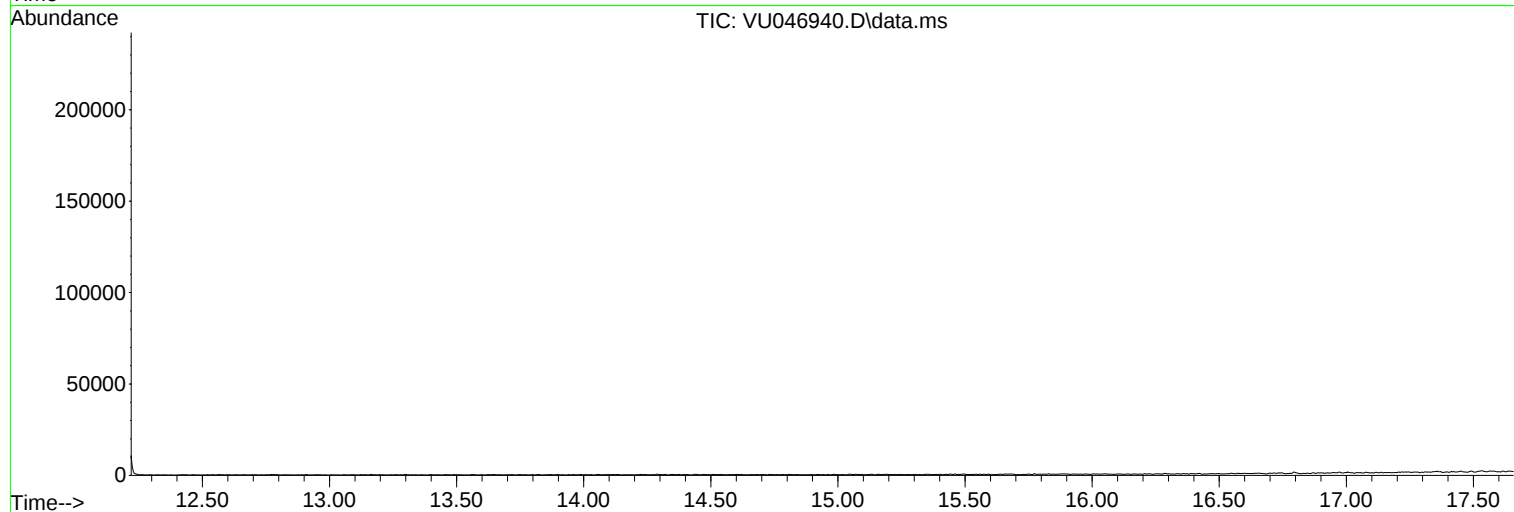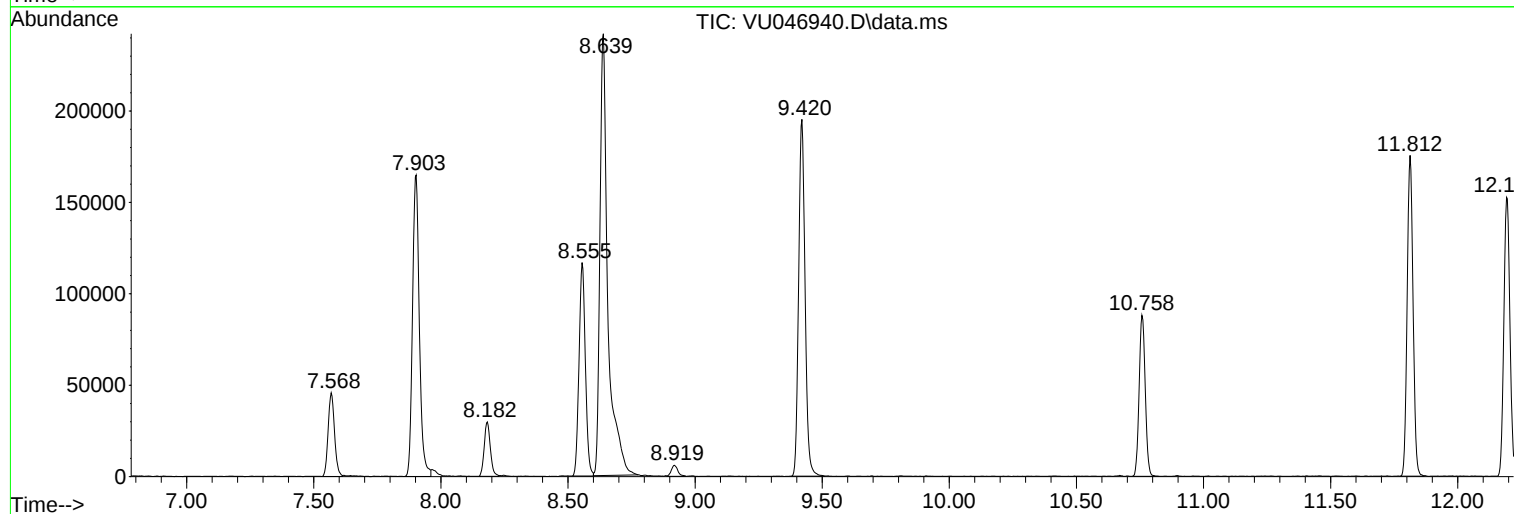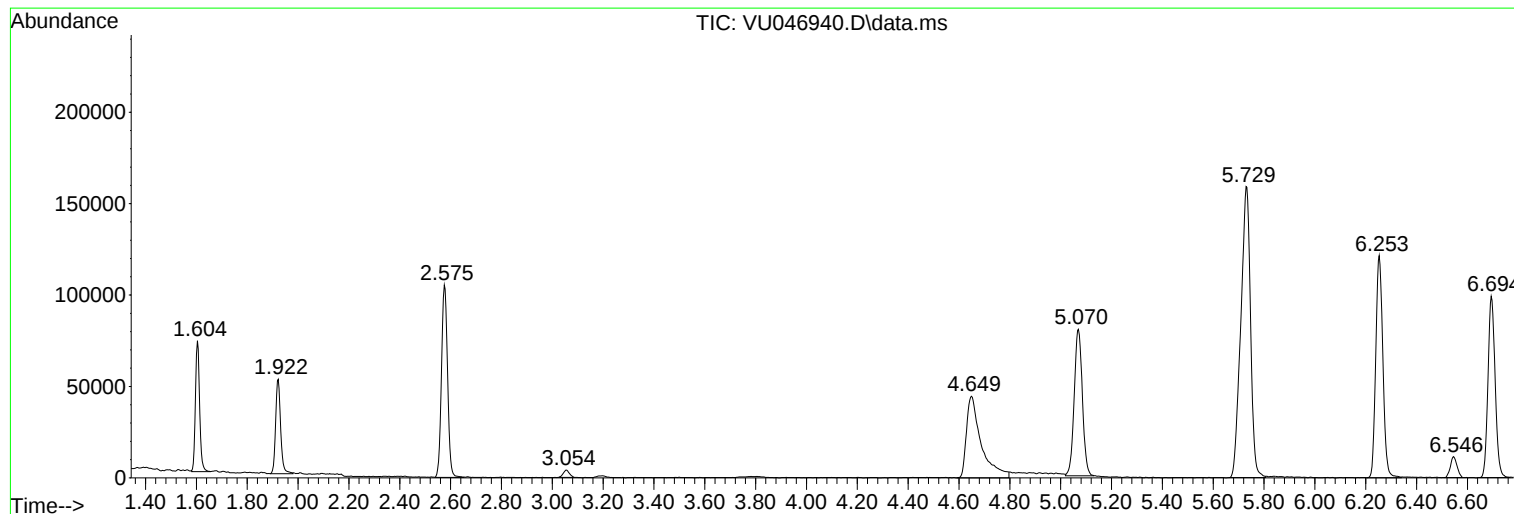

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046940.D
Acq On : 01 Feb 2022 00:48
Operator : SY/MD
Sample : N1328-14DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HN3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046940.D
Acq On : 01 Feb 2022 00:48
Operator : SY/MD
Sample : N1328-14DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HN3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc