

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
 Data File : VU046945.D
 Acq On : 01 Feb 2022 02:50
 Operator : SY/MD
 Sample : N1328-01DL2 1000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHM0DL2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU046945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	96	rVB	73270	84911	16.06%	2.067%
2	1.919	172	180	201	rVB	51797	70006	13.24%	1.704%
3	2.578	371	385	404	rBV4	133257	254453	48.12%	6.194%
4	3.054	524	533	543	rBV2	3122	5603	1.06%	0.136%
5	4.658	1015	1032	1077	rBV	47379	207178	39.18%	5.043%
6	5.070	1143	1160	1178	rVB	80153	174622	33.03%	4.250%
7	5.324	1225	1239	1250	rBV4	3027	6289	1.19%	0.153%
8	5.729	1344	1365	1395	rBV2	158529	421647	79.75%	10.263%
9	6.253	1511	1528	1546	rBV	122534	239256	45.25%	5.824%
10	6.546	1606	1619	1637	rBV	178779	334778	63.32%	8.149%
11	6.693	1650	1665	1683	rBV	96499	191758	36.27%	4.668%
12	7.568	1922	1937	1952	rBV	44252	79742	15.08%	1.941%
13	7.902	2027	2041	2060	rBV	166812	309204	58.48%	7.526%
14	8.182	2117	2128	2142	rBV2	29639	50143	9.48%	1.221%
15	8.555	2233	2244	2258	rBV2	70911	122988	23.26%	2.994%
16	8.639	2258	2270	2309	rVB	241749	528734	100.00%	12.870%
17	8.915	2348	2356	2371	rBV2	6084	10888	2.06%	0.265%
18	9.420	2500	2513	2535	rBV	195856	339220	64.16%	8.257%
19	10.758	2918	2929	2947	rVB	87628	145490	27.52%	3.541%
20	11.812	3245	3257	3277	rBV	174872	282183	53.37%	6.869%
21	12.195	3364	3376	3397	rVB	154413	249218	47.13%	6.066%




Sum of corrected areas: 4108311

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046945.D
Acq On : 01 Feb 2022 02:50
Operator : SY/MD
Sample : N1328-01DL2 1000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHM0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

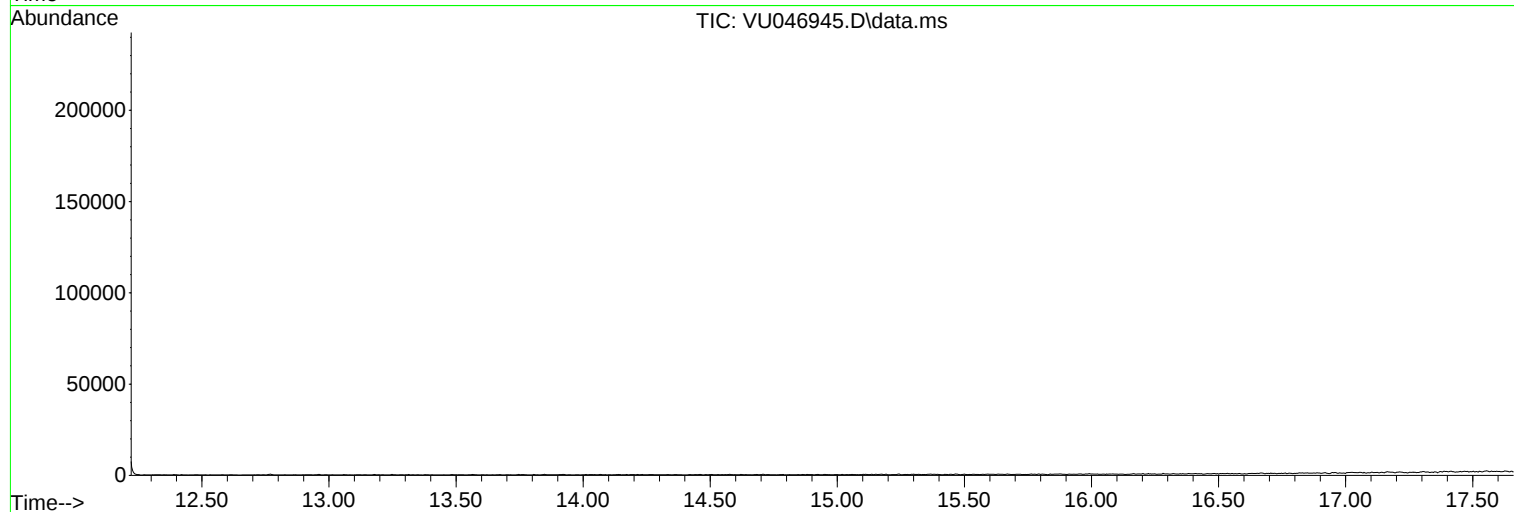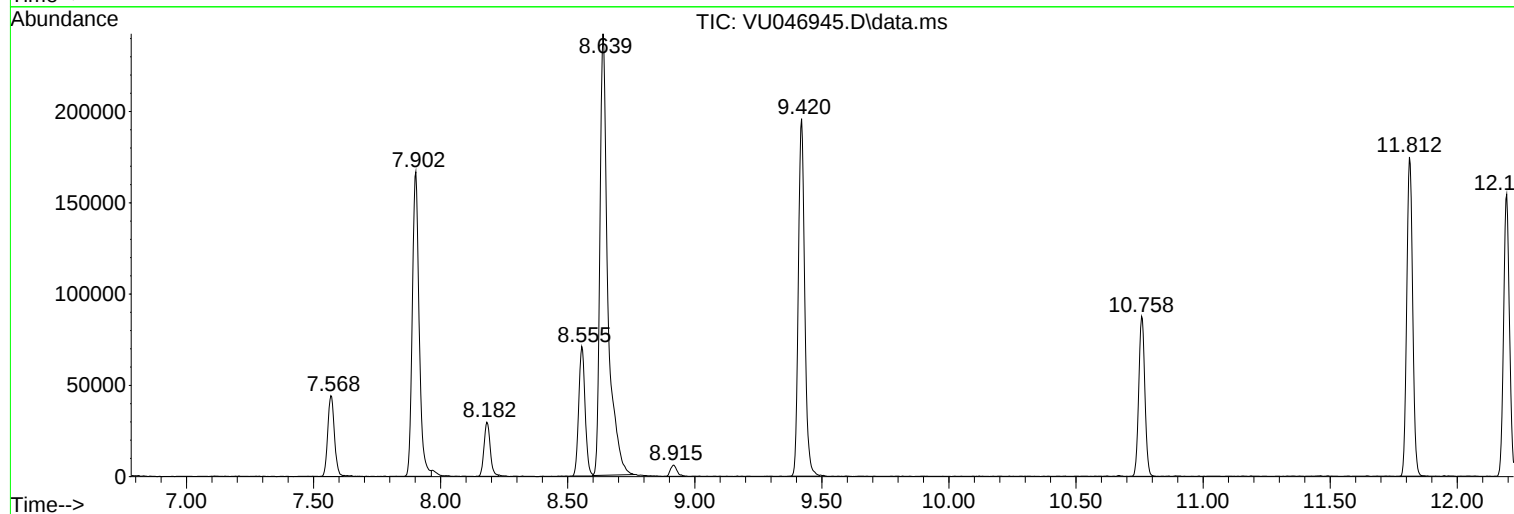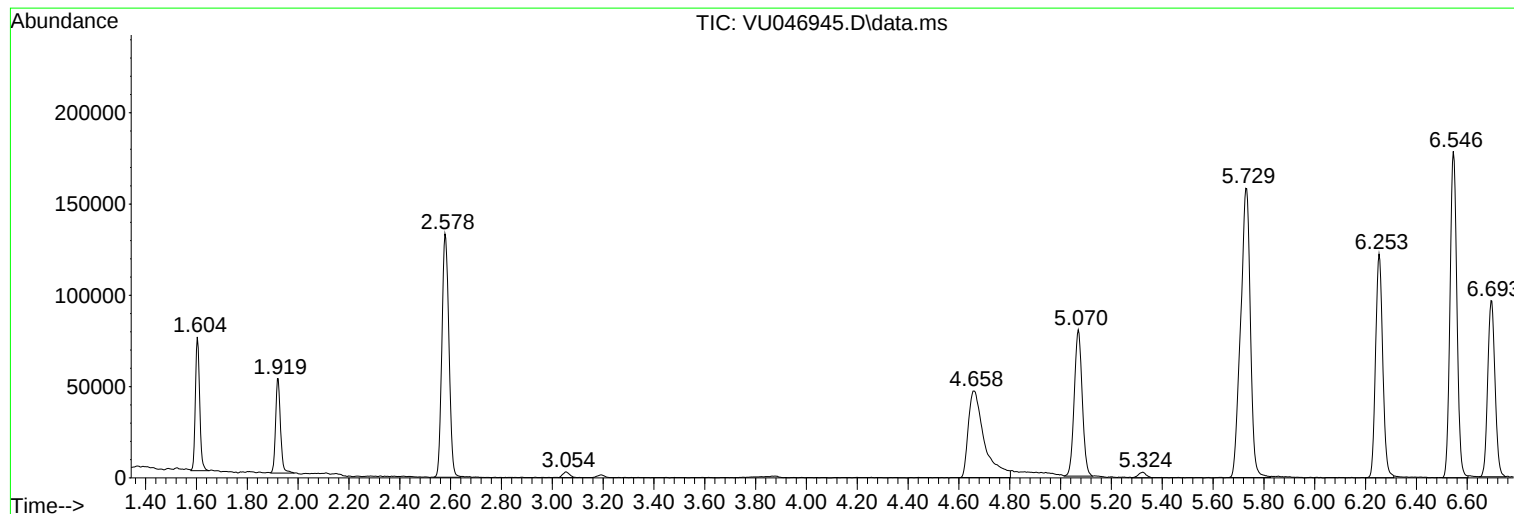

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046945.D
Acq On : 01 Feb 2022 02:50
Operator : SY/MD
Sample : N1328-01DL2 1000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HM0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046945.D
Acq On : 01 Feb 2022 02:50
Operator : SY/MD
Sample : N1328-01DL2 1000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHM0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc