

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
 Data File : VU046948.D
 Acq On : 01 Feb 2022 04:03
 Operator : SY/MD
 Sample : N1273-18DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HL6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	93	rVB	68364	77019	14.26%	1.972%
2	1.919	172	180	191	rBV	50298	67804	12.56%	1.736%
3	2.575	369	384	401	rBV2	107344	189364	35.07%	4.848%
4	4.662	1014	1033	1074	rBV3	56542	232060	42.98%	5.941%
5	5.070	1145	1160	1183	rVB2	80121	179200	33.19%	4.587%
6	5.321	1228	1238	1250	rVB4	2834	5921	1.10%	0.152%
7	5.732	1343	1366	1389	rBV3	157355	419536	77.69%	10.740%
8	6.253	1514	1528	1559	rBV	122298	236065	43.72%	6.043%
9	6.546	1607	1619	1635	rVB2	53695	99663	18.46%	2.551%
10	6.694	1651	1665	1682	rBV	99466	192785	35.70%	4.935%
11	7.568	1924	1937	1960	rBV	45526	79591	14.74%	2.037%
12	7.903	2025	2041	2060	rBV	159710	296000	54.82%	7.577%
13	8.182	2116	2128	2142	rBV	28311	48969	9.07%	1.254%
14	8.555	2232	2244	2258	rBV	128287	221855	41.09%	5.679%
15	8.639	2258	2270	2313	rVB	244184	539980	100.00%	13.823%
16	8.915	2347	2356	2372	rVB2	6252	10866	2.01%	0.278%
17	9.420	2500	2513	2539	rBV	189206	337513	62.50%	8.640%
18	10.758	2918	2929	2945	rVB	89069	145592	26.96%	3.727%
19	11.812	3245	3257	3275	rBV	175297	279763	51.81%	7.162%
20	12.195	3361	3376	3395	rBV	150125	246821	45.71%	6.318%




Sum of corrected areas: 3906367

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046948.D
Acq On : 01 Feb 2022 04:03
Operator : SY/MD
Sample : N1273-18DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

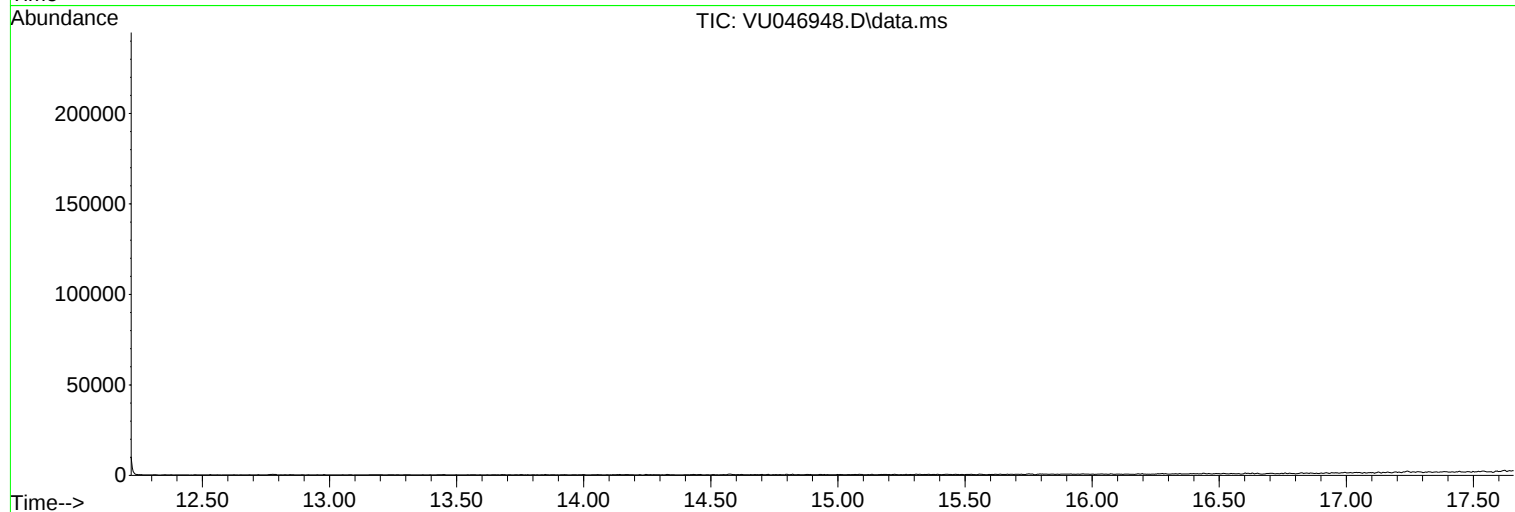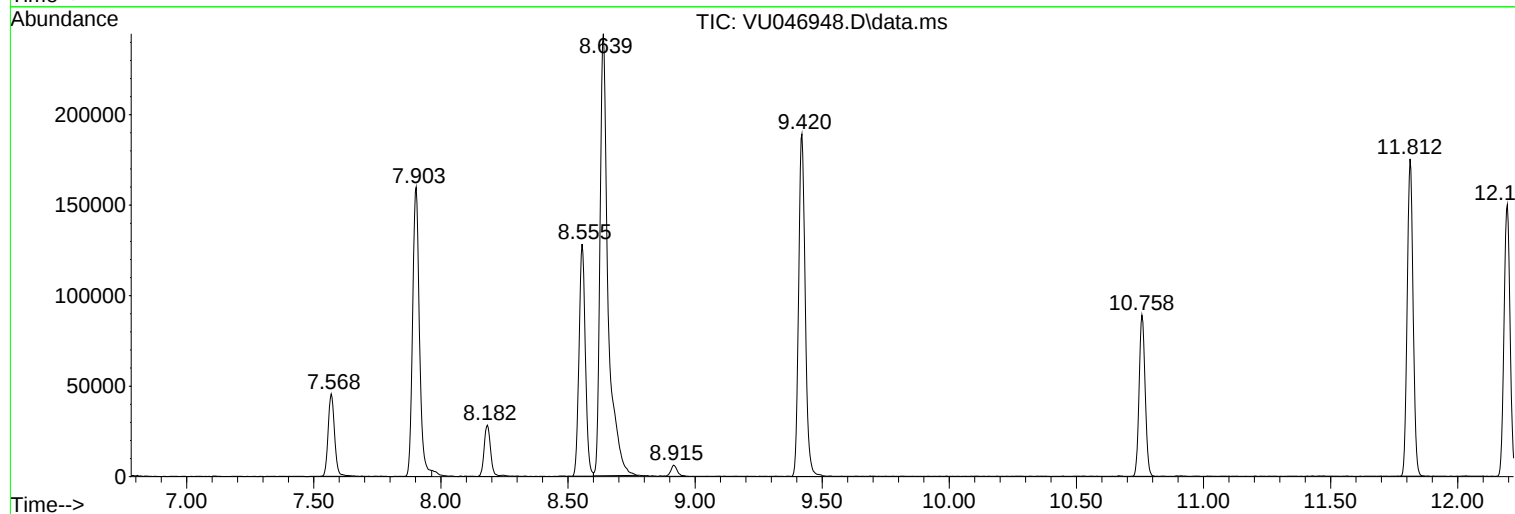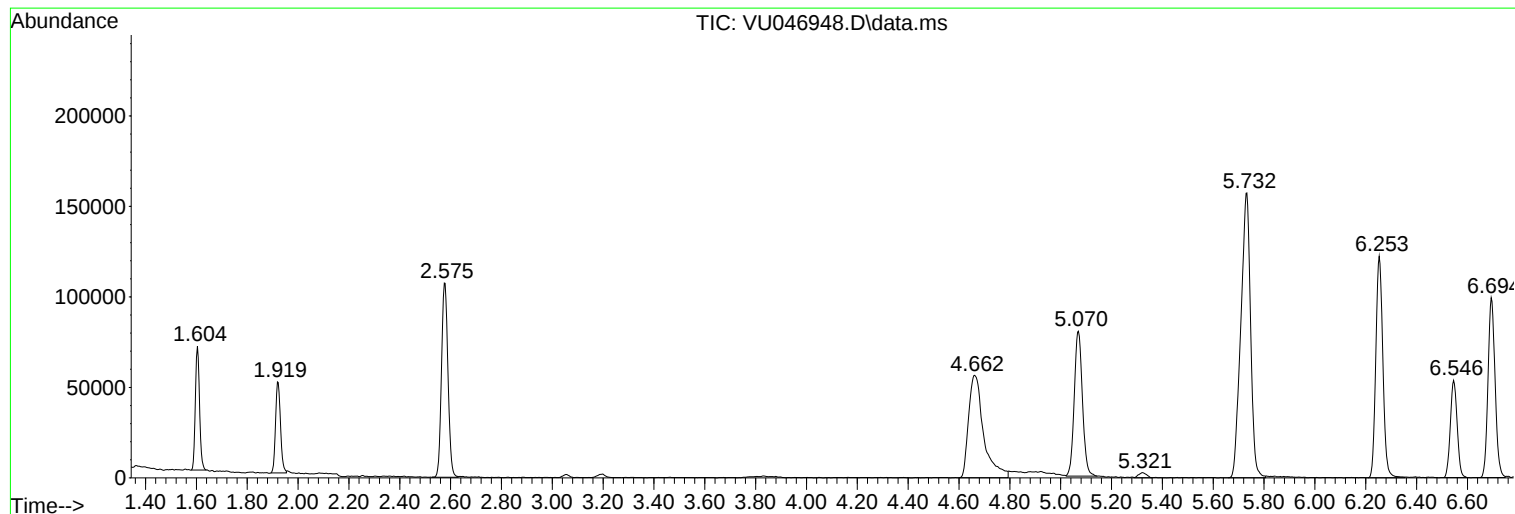

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046948.D
Acq On : 01 Feb 2022 04:03
Operator : SY/MD
Sample : N1273-18DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046948.D
Acq On : 01 Feb 2022 04:03
Operator : SY/MD
Sample : N1273-18DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc