

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
 Data File : VU046950.D
 Acq On : 01 Feb 2022 04:51
 Operator : SY/MD
 Sample : N1273-21 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHL9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU046950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.607	74	83	96	rBV2	53245	66343	9.52%	1.350%
2	1.922	172	181	200	rVB	38426	52485	7.53%	1.068%
3	2.588	372	388	406	rBV4	322383	577807	82.88%	11.759%
4	3.195	563	577	588	rVB2	4256	9564	1.37%	0.195%
5	3.880	773	790	809	rVB3	7982	19138	2.75%	0.389%
6	4.671	1013	1036	1063	rBV4	149100	449889	64.53%	9.156%
7	5.070	1142	1160	1181	rVB	70270	159102	22.82%	3.238%
8	5.729	1344	1365	1393	rBV2	129168	352608	50.58%	7.176%
9	6.253	1514	1528	1551	rBV	100680	194572	27.91%	3.960%
10	6.546	1605	1619	1638	rBV	372532	697129	100.00%	14.187%
11	6.694	1652	1665	1681	rVB	88807	170904	24.52%	3.478%
12	7.568	1926	1937	1952	rBV	34145	60316	8.65%	1.227%
13	7.903	2028	2041	2058	rBV	119185	222818	31.96%	4.535%
14	8.182	2118	2128	2148	rBV2	22089	38250	5.49%	0.778%
15	8.555	2232	2244	2259	rBV	249978	432886	62.10%	8.810%
16	8.639	2259	2270	2317	rVB	235480	576123	82.64%	11.725%
17	9.420	2501	2513	2545	rVB	154934	272558	39.10%	5.547%
18	10.758	2917	2929	2945	rBV	89344	148231	21.26%	3.017%
19	11.812	3243	3257	3274	rVB	132426	215353	30.89%	4.383%
20	12.195	3364	3376	3390	rBV	121531	197706	28.36%	4.023%




Sum of corrected areas: 4913782

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046950.D
Acq On : 01 Feb 2022 04:51
Operator : SY/MD
Sample : N1273-21 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

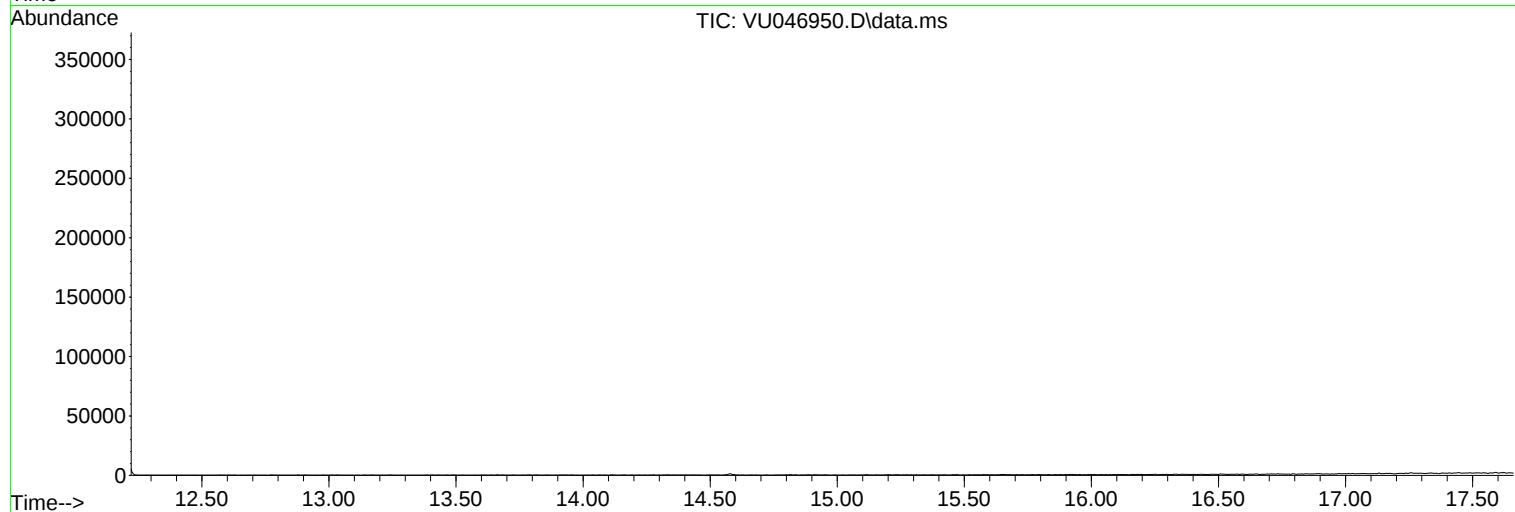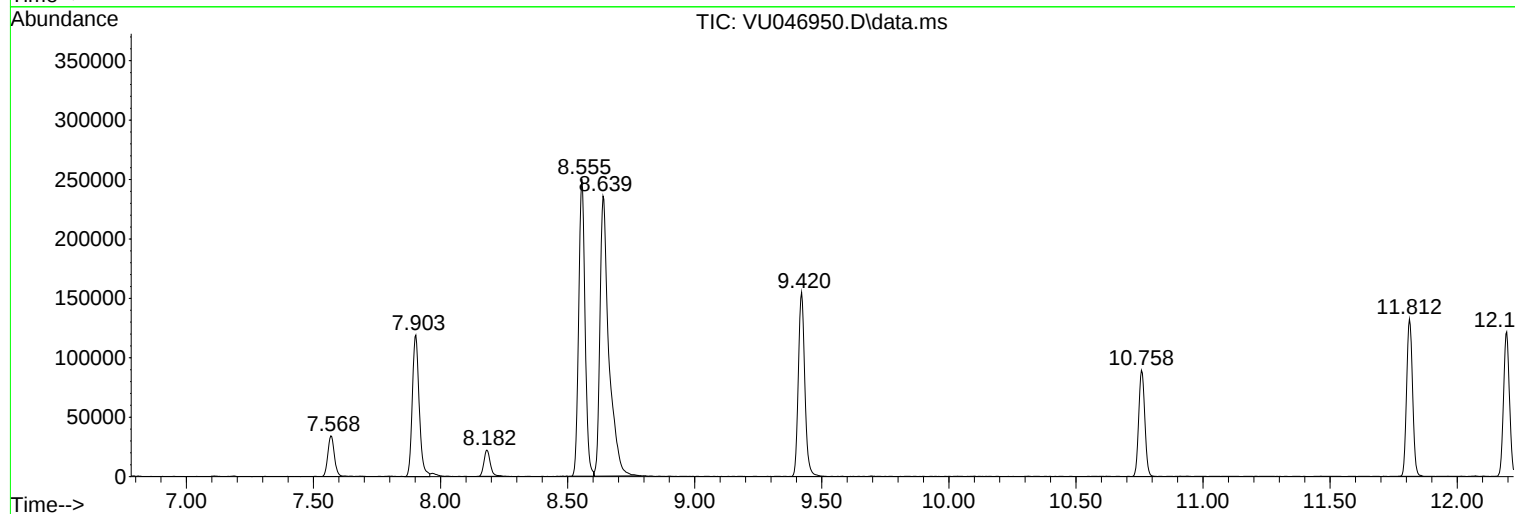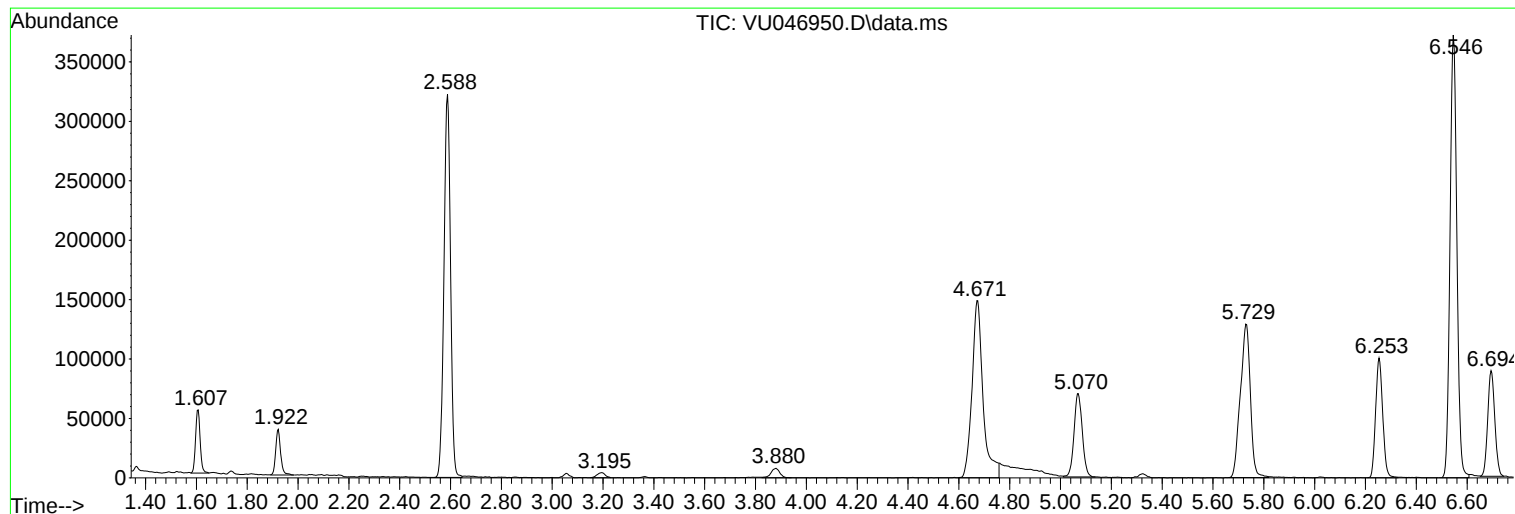

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046950.D
Acq On : 01 Feb 2022 04:51
Operator : SY/MD
Sample : N1273-21 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
Data File : VU046950.D
Acq On : 01 Feb 2022 04:51
Operator : SY/MD
Sample : N1273-21 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
