
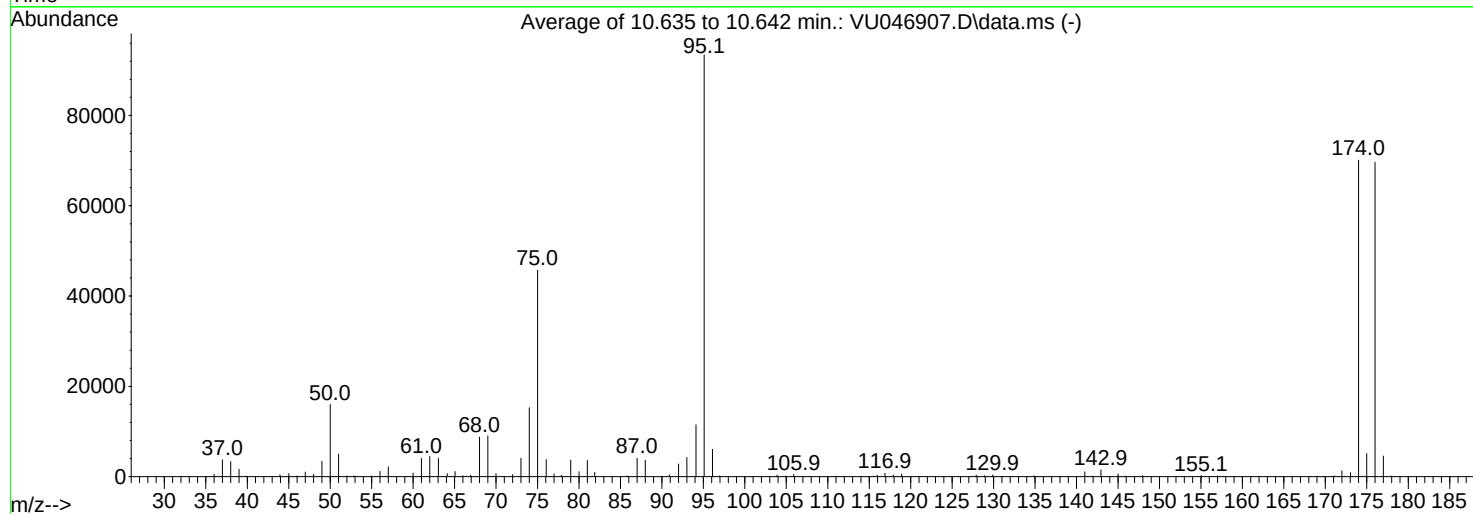


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU013122\
 Data File : VU046907.D
 Acq On : 31 Jan 2022 08:59
 Operator : SY/MD
 Sample : BFB050
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB050

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Feb 03 02:56:36 2022

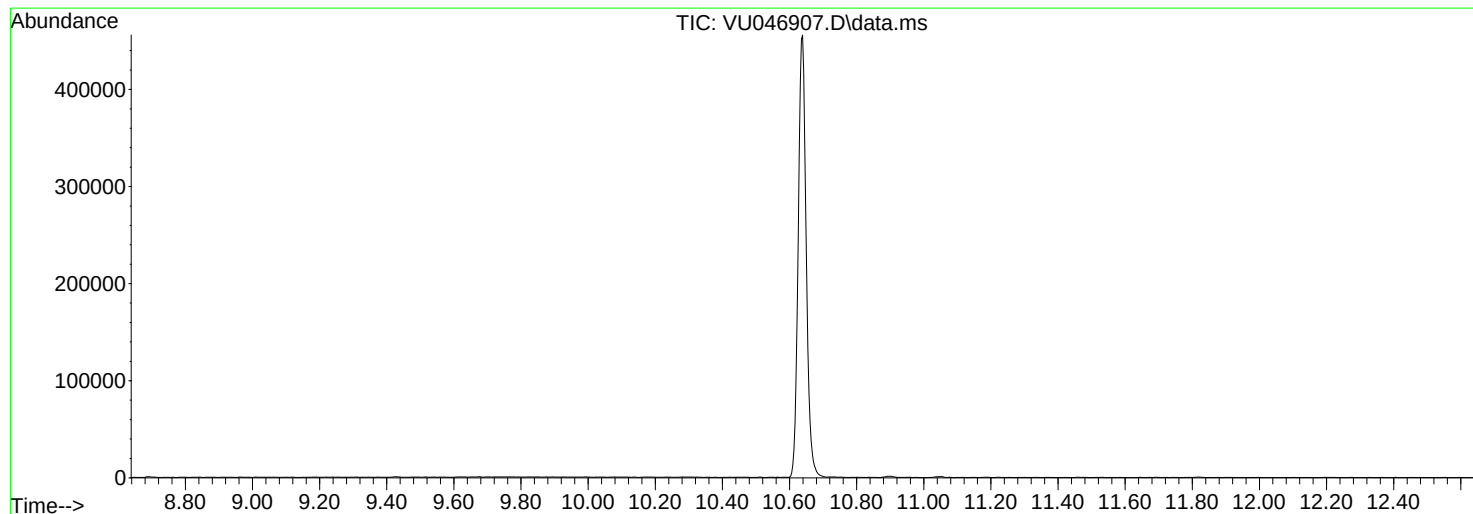

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	15973	PASS
75	95	30	80	48.9	45712	PASS
95	95	100	100	100.0	93413	PASS
96	95	5	9	6.5	6063	PASS
173	174	0.00	2	1.3	891	PASS
174	95	50	120	75.0	70088	PASS
175	174	5	9	7.3	5101	PASS
176	174	95	101	99.3	69621	PASS
177	176	5	9	6.6	4580	PASS

m/z	Abundance
36.00	331.0
38.00	157.0
43.90	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB050

m/z	Abundance
36.00	912.0
37.00	4032.0
38.00	3619.0
39.00	1723.0
39.90	129.0
44.00	528.0
45.00	708.0
46.00	138.0
47.00	1129.0
48.00	571.0
49.00	3585.0
50.00	16592.0
51.00	5339.0
51.90	234.0
52.90	156.0
54.90	197.0
56.00	1163.0
57.00	2344.0
60.00	829.0
61.00	4093.0
62.00	4676.0
63.10	4282.0
64.10	778.0
65.10	1206.0
66.00	181.0
67.00	207.0
68.00	8968.0
69.00	9446.0
70.00	654.0
72.00	434.0
73.00	4187.0
74.00	15645.0
75.00	47008.0
76.00	3922.0
77.00	603.0
77.90	339.0
79.00	3974.0
80.00	1121.0
81.00	3796.0
81.90	1016.0
85.80	215.0
87.00	4198.0
88.00	3845.0
90.90	399.0
92.00	2925.0
93.00	4465.0
94.10	11834.0
95.10	94696.0
96.10	6321.0
97.00	159.0
103.90	396.0
104.90	163.0
105.90	512.0
110.90	101.0
115.90	329.0
116.90	806.0
117.90	308.0
118.90	577.0
123.90	122.0
127.90	401.0
128.90	223.0
129.90	405.0
134.90	204.0
137.00	113.0
141.00	1047.0
141.90	106.0
142.90	1602.0
143.90	106.0
145.00	636.0
145.90	166.0
148.00	215.0
155.00	208.0
157.00	193.0
171.10	223.0
172.00	1257.0
173.10	986.0
174.00	70456.0
175.00	5126.0
176.00	69952.0
177.00	4737.0
177.90	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB050

m/z	Abundance
36.00	854.0
37.00	3838.0
38.00	3606.0
39.00	1688.0
39.80	155.0
44.00	581.0
45.00	694.0
45.90	154.0
47.00	1085.0
48.00	563.0
49.00	3539.0
50.00	16488.0
51.00	5154.0
52.00	178.0
52.90	175.0
55.00	192.0
56.00	1233.0
57.00	2278.0
60.00	803.0
61.00	4175.0
62.00	4652.0
63.00	4148.0
64.10	709.0
65.00	1172.0
66.00	234.0
66.90	291.0
68.00	8975.0
69.00	9207.0
70.00	699.0
72.00	457.0
73.00	4218.0
74.00	15623.0
75.00	47088.0
76.00	3925.0
77.00	640.0
77.90	286.0
79.00	3807.0
80.00	1129.0
81.00	3715.0
81.90	975.0
85.80	198.0
87.00	4263.0
88.00	3725.0
90.90	422.0
92.00	2893.0
93.00	4380.0
94.10	11864.0
95.10	96504.0
96.10	6262.0
96.90	166.0
103.90	371.0
104.90	170.0
105.90	503.0
111.00	113.0
115.90	348.0
116.90	776.0
117.90	356.0
118.90	562.0
127.90	357.0
128.90	240.0
129.90	431.0
130.90	106.0
134.90	172.0
137.00	102.0
141.00	1084.0
141.90	135.0
143.00	1530.0
145.00	631.0
145.90	148.0
148.00	269.0
155.10	239.0
157.00	206.0
159.10	101.0
161.10	114.0
171.10	178.0
172.00	1356.0
173.00	903.0
174.00	72240.0
175.00	5282.0
176.00	71952.0
177.00	4771.0
177.90	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB050

m/z	Abundance
36.00	797.0
37.00	3320.0
38.00	3265.0
39.00	1540.0
39.90	167.0
44.00	616.0
45.00	601.0
45.90	152.0
47.00	899.0
48.00	402.0
49.00	3096.0
50.00	14839.0
51.00	4473.0
52.10	134.0
52.80	174.0
55.00	176.0
56.00	1178.0
57.00	2000.0
60.00	750.0
61.00	3872.0
62.00	4115.0
63.00	3689.0
64.10	574.0
65.00	1084.0
66.00	207.0
66.90	321.0
68.00	8278.0
69.00	8487.0
70.00	650.0
72.00	485.0
73.00	3829.0
74.00	14517.0
75.00	43040.0
76.10	3503.0
77.00	613.0
77.90	277.0
79.00	3287.0
80.00	1007.0
81.00	3286.0
81.90	855.0
85.80	154.0
87.00	3737.0
88.00	3401.0
90.90	359.0
92.00	2551.0
93.00	3899.0
94.10	10792.0
95.10	89040.0
96.10	5606.0
96.90	163.0
103.90	323.0
104.90	139.0
105.90	455.0
111.10	106.0
115.00	101.0
116.00	346.0
116.90	641.0
117.90	362.0
118.90	543.0
127.90	284.0
128.90	215.0
129.90	373.0
130.90	137.0
134.90	142.0
136.90	110.0
141.00	1032.0
141.90	159.0
143.00	1323.0
145.00	553.0
145.90	128.0
147.90	256.0
155.10	250.0
157.00	181.0
161.10	101.0
170.90	161.0
172.00	1296.0
173.00	783.0
174.00	67568.0
175.00	4895.0
176.00	66960.0
177.00	4231.0
177.90	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB050