

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
 Data File : VU046997.D
 Acq On : 02 Feb 2022 13:27
 Operator : SY/MD
 Sample : N1348-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Feb 03 02:59:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 03 02:56:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	103664	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	121009	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	52464	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	47684	5.428	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	108.600%
7) Chloroethane-d5	1.919	69	38503	5.563	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.200%
11) 1,1-Dichloroethene-d2	2.575	65	18060	5.169	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	103.400%
20) 2-Butanone-d5	4.639	46	112630	43.281	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.560%
24) Chloroform-d	5.070	84	77595	5.032	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.600%
26) 1,2-Dichloroethane-d4	5.707	65	42127	5.017	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
32) Benzene-d6	5.732	84	151545	4.261	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.200%
36) 1,2-Dichloropropane-d6	6.694	67	49228	4.610	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.200%
41) Toluene-d8	7.903	98	116406	3.576	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.600%
43) trans-1,3-Dichloroprop...	8.182	79	17238	3.676	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.600%
46) 2-Hexanone-d5	8.636	63	89969	32.401	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	64.800%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	43178	4.028	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.600%
66) 1,2-Dichlorobenzene-d4	12.195	152	43056	4.376	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.600%
Target Compounds						Qvalue
3) Chloromethane	1.523	50	2874	0.358	ug/L	93
13) Acetone	2.665	43	5864	4.143	ug/L	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU046997.D
Acq On : 02 Feb 2022 13:27
Operator : SY/MD
Sample : N1348-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Feb 03 02:59:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 03 02:56:36 2022
Response via : Initial Calibration




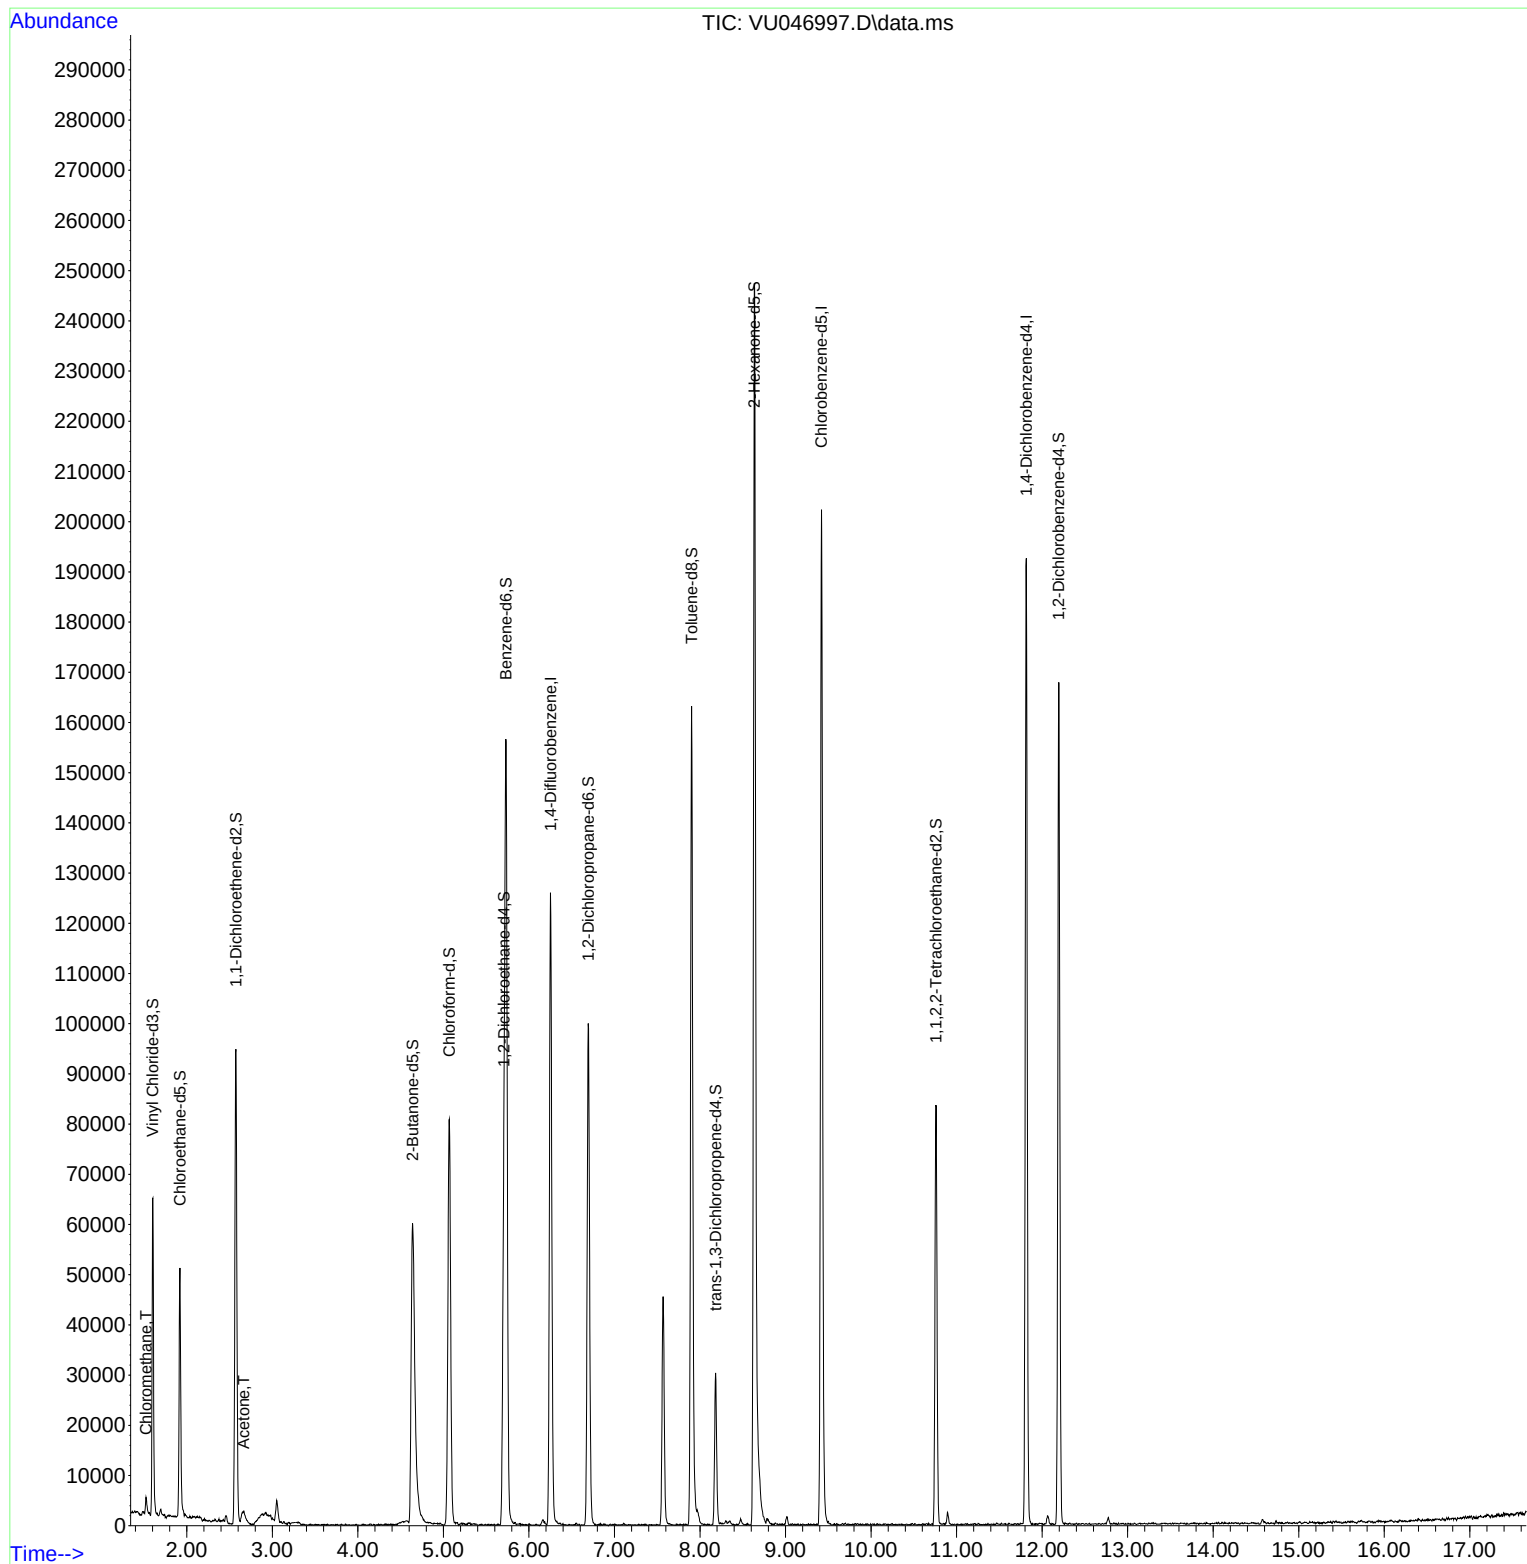


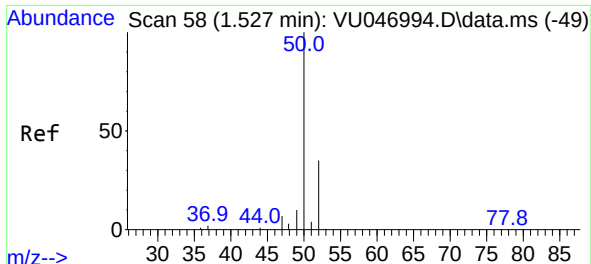

#3
Chloromethane
Concen: 0.358 ug/L
RT: 1.523 min Scan# 51
Delta R.T. -0.003 min
Lab File: VU046997.D
Acq: 02 Feb 2022 13:27

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Tgt Ion: 50 Resp: 2874
Ion Ratio Lower Upper
50 100
52 28.8 23.0 42.8

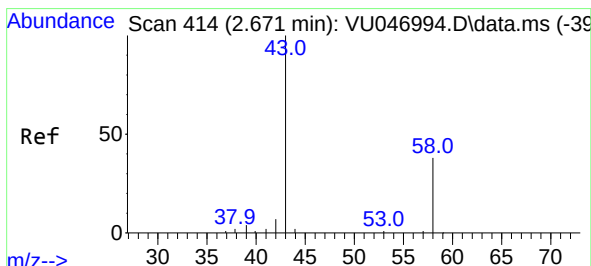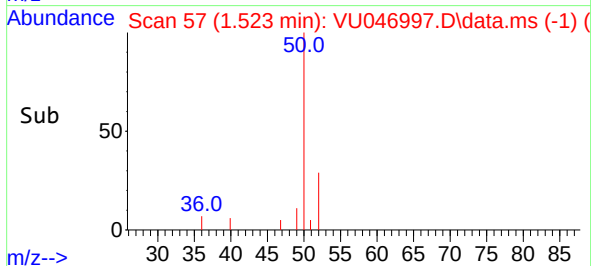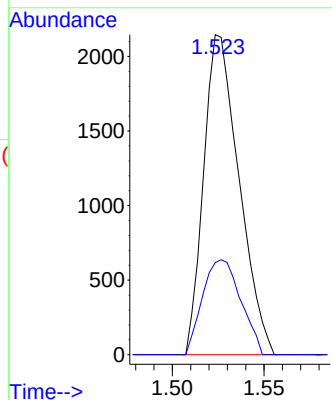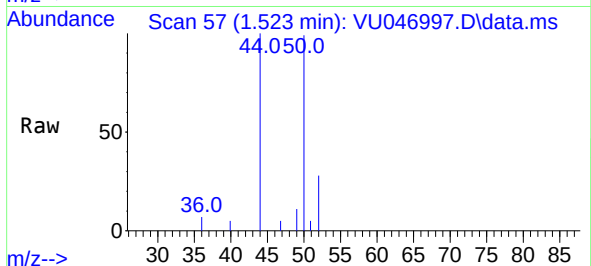

#13
Acetone
Concen: 4.143 ug/L
RT: 2.665 min Scan# 412
Delta R.T. -0.006 min
Lab File: VU046997.D
Acq: 02 Feb 2022 13:27

Tgt Ion: 43 Resp: 5864
Ion Ratio Lower Upper
43 100
58 16.1 0.0 71.6

