

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
 Data File : VU046998.D
 Acq On : 02 Feb 2022 13:51
 Operator : SY/MD
 Sample : N1349-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHP0

Quant Time: Feb 03 03:00:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 03 02:56:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	102523	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	119157	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	51646	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	45696	5.260	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	105.200%	
7) Chloroethane-d5	1.919	69	37195	5.434	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	108.600%	
11) 1,1-Dichloroethene-d2	2.571	65	17166	4.967	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	99.400%	
20) 2-Butanone-d5	4.636	46	107620	41.816	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	83.640%	
24) Chloroform-d	5.070	84	76349	5.006	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.200%	
26) 1,2-Dichloroethane-d4	5.706	65	40952	4.931	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.600%	
32) Benzene-d6	5.732	84	146348	4.179	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.600%	
36) 1,2-Dichloropropane-d6	6.694	67	47457	4.513	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.200%	
41) Toluene-d8	7.902	98	115021	3.588	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	71.800%	
43) trans-1,3-Dichloroprop...	8.182	79	17685	3.830	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	76.600%	
46) 2-Hexanone-d5	8.636	63	83883	30.679	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	61.360%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	41758	3.956	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	79.200%	
66) 1,2-Dichlorobenzene-d4	12.195	152	42198	4.357	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	87.200%	
Target Compounds						Qvalue
3) Chloromethane	1.527	50	6049	0.762	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU046998.D
Acq On : 02 Feb 2022 13:51
Operator : SY/MD
Sample : N1349-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP0

Quant Time: Feb 03 03:00:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 03 02:56:36 2022
Response via : Initial Calibration

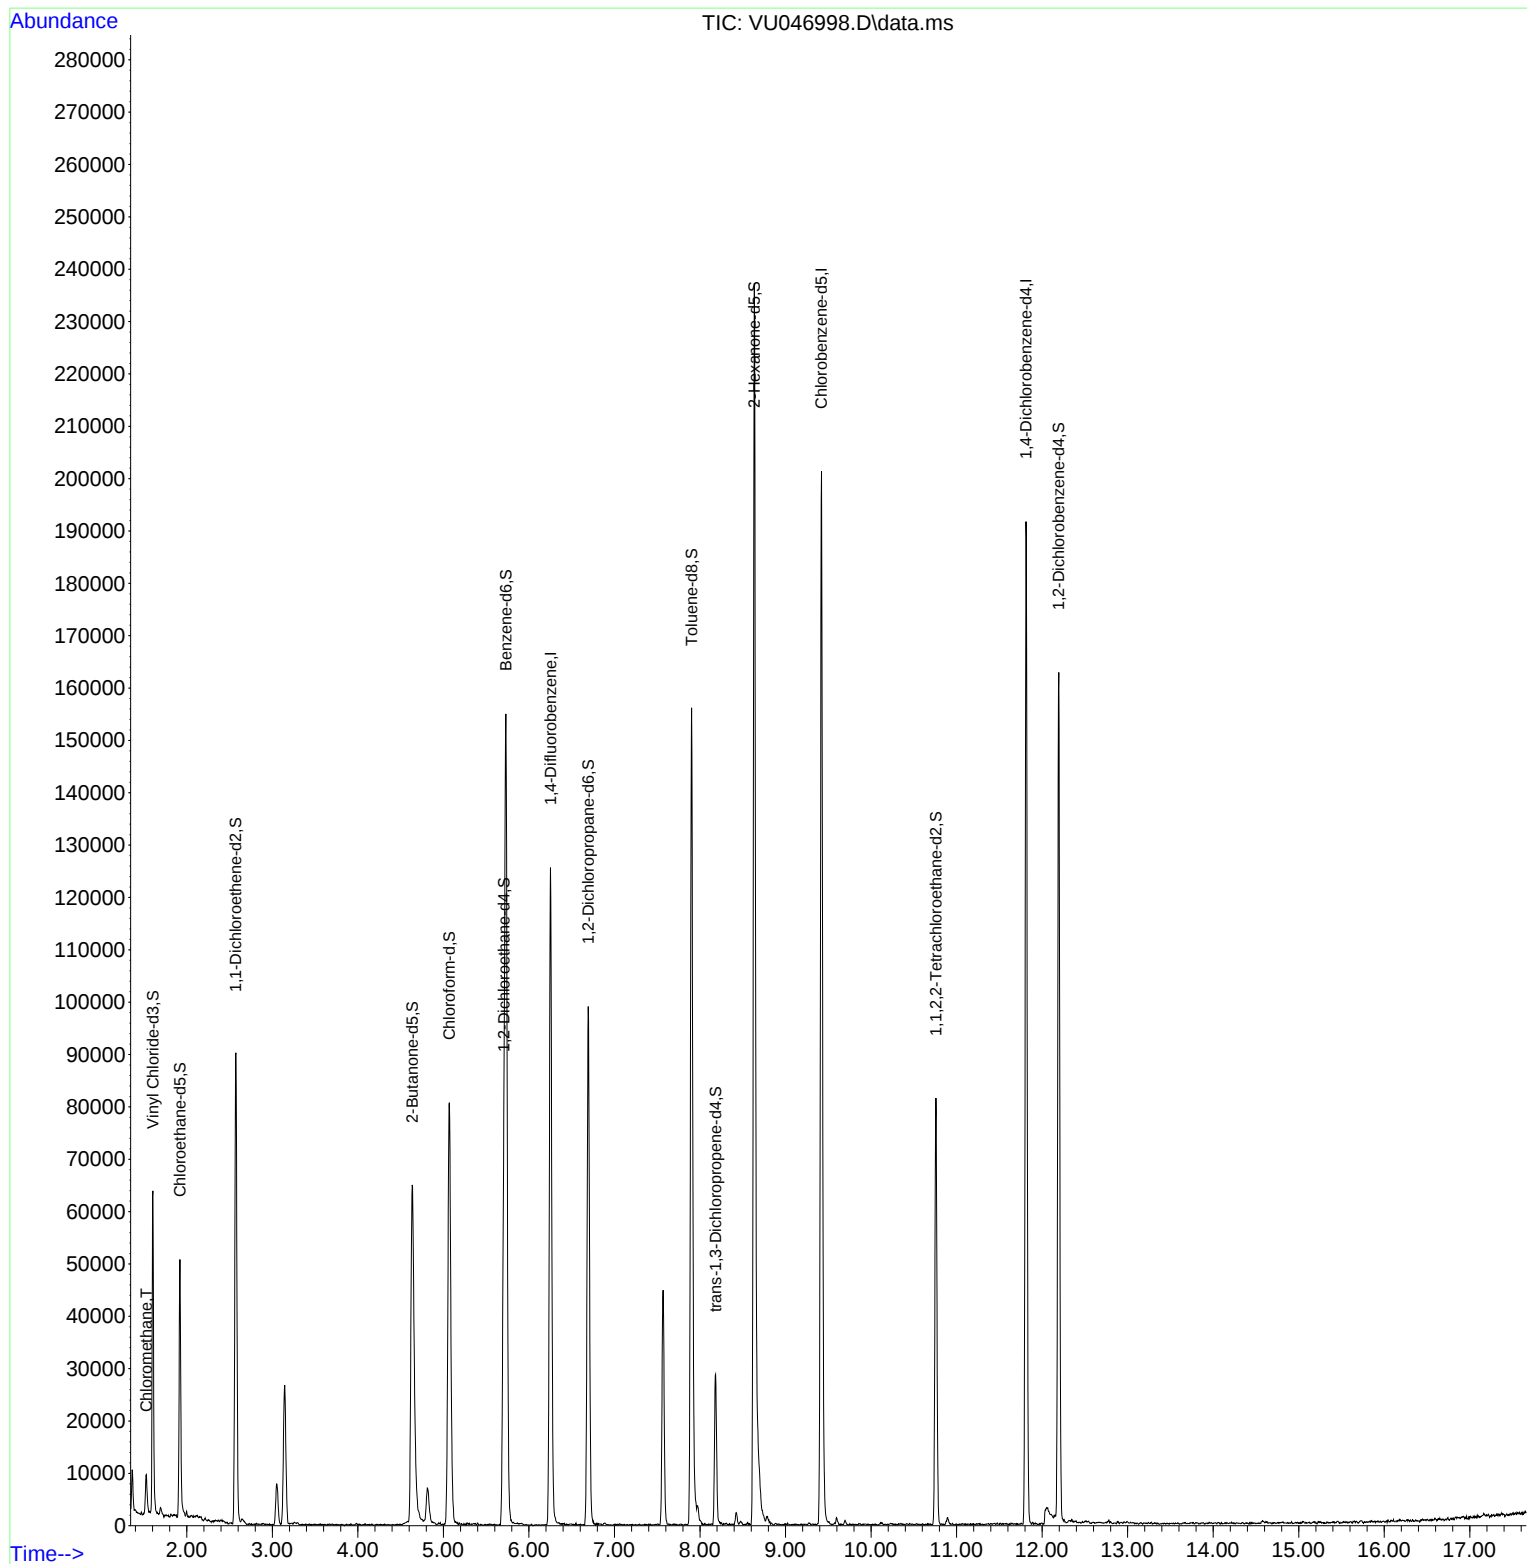

Abundance Scan 58 (1.527 min): VU046994.D\data.ms (-49)

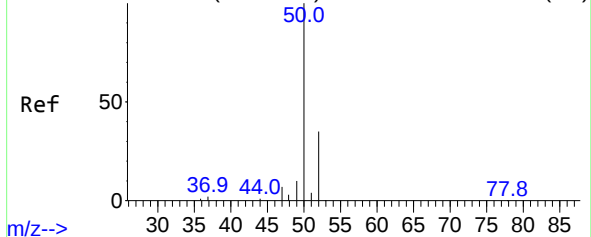

#3

Chloromethane

Concen: 0.762 ug/L

RT: 1.527 min Scan# 58

Delta R.T. -0.000 min

Lab File: VU046998.D

Acq: 02 Feb 2022 13:51


Instrument :

MSVOA_U

ClientSampleId :

COHP0

Abundance Scan 58 (1.527 min): VU046998.D\data.ms

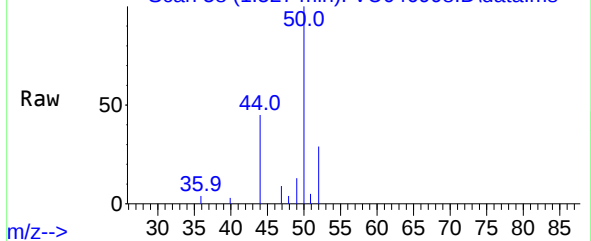


Tgt Ion: 50 Resp: 6049

Ion Ratio Lower Upper

50 100

52 29.0 23.0 42.8

Abundance

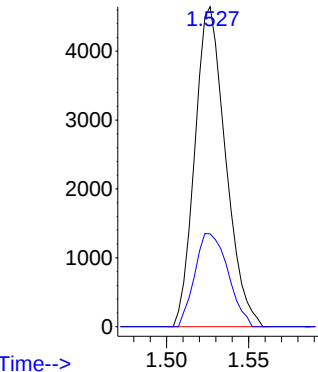

Abundance Scan 58 (1.527 min): VU046998.D\data.ms (-1) (

