

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
 Data File : VU047001.D
 Acq On : 02 Feb 2022 15:03
 Operator : SY/MD
 Sample : N1349-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HQ1

Quant Time: Feb 03 03:00:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 03 02:56:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	98304	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	116581	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	49949	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	42699	5.126	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	102.600%	
7) Chloroethane-d5	1.919	69	35692	5.438	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	108.800%	
11) 1,1-Dichloroethene-d2	2.572	65	16093	4.857	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	97.200%	
20) 2-Butanone-d5	4.636	46	100113	40.569	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	81.140%	
24) Chloroform-d	5.067	84	71748	4.906	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.200%	
26) 1,2-Dichloroethane-d4	5.703	65	38383	4.820	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.400%	
32) Benzene-d6	5.732	84	139630	4.075	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	81.600%	
36) 1,2-Dichloropropane-d6	6.694	67	45039	4.378	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	87.600%	
41) Toluene-d8	7.903	98	106754	3.404	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	68.000%#	
43) trans-1,3-Dichloroprop...	8.182	79	15630	3.460	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	69.200%	
46) 2-Hexanone-d5	8.636	63	77176	28.849	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	57.700%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	37761	3.656	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	73.200%	
66) 1,2-Dichlorobenzene-d4	12.195	152	39913	4.261	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	85.200%	
Target Compounds						Qvalue
3) Chloromethane	1.527	50	7012	0.921	ug/L	96
13) Acetone	2.655	43	5503	4.100	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU047001.D
Acq On : 02 Feb 2022 15:03
Operator : SY/MD
Sample : N1349-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HQ1

Quant Time: Feb 03 03:00:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 03 02:56:36 2022
Response via : Initial Calibration




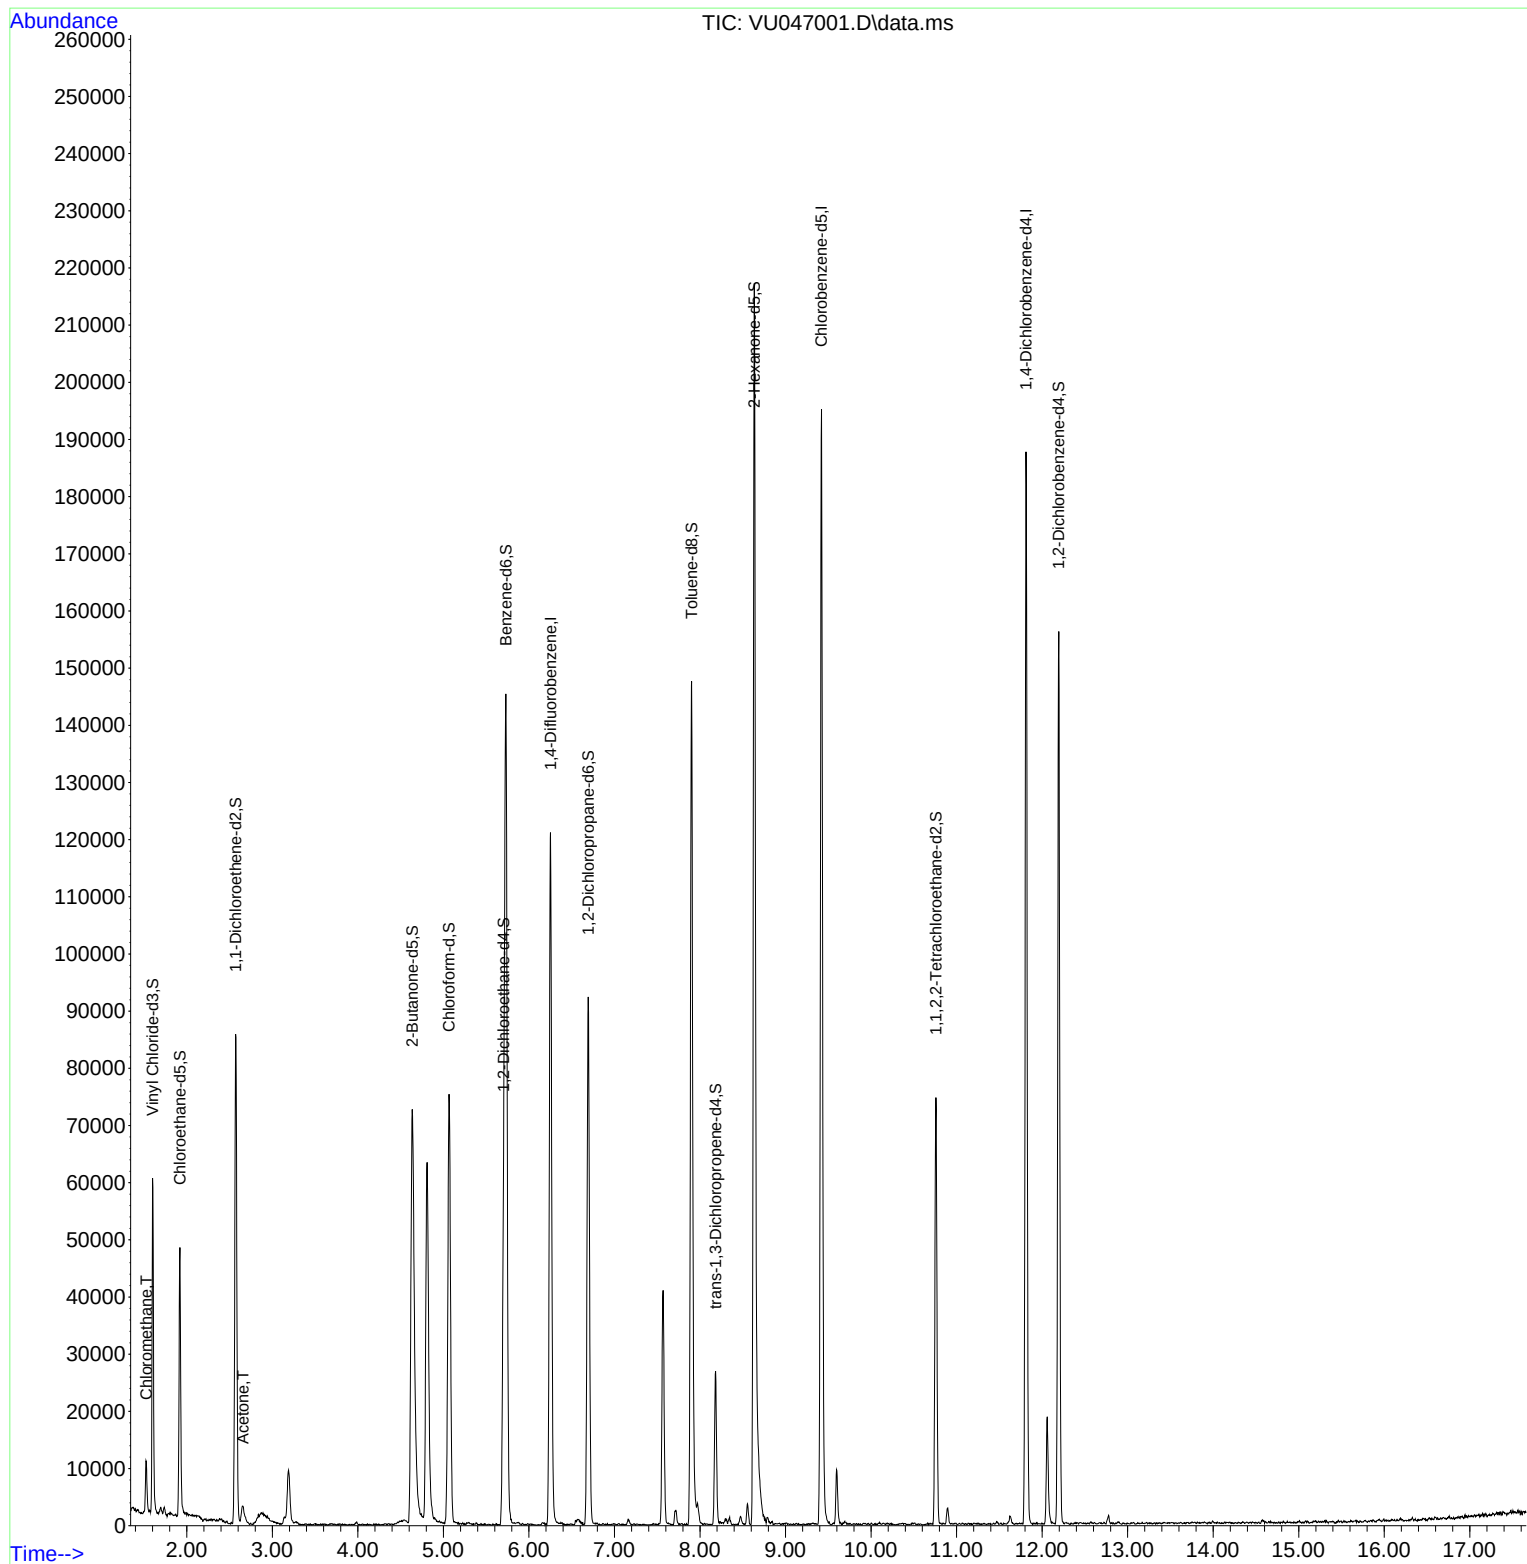


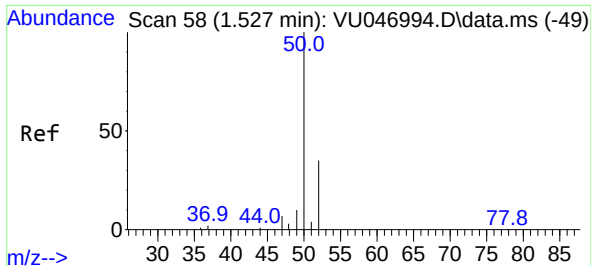

#3
Chloromethane
Concen: 0.921 ug/L
RT: 1.527 min Scan# 50
Delta R.T. -0.000 min
Lab File: VU047001.D
Acq: 02 Feb 2022 15:03

Instrument :
MSVOA_U
ClientSampleId :
C0HQ1

Tgt Ion: 50 Resp: 7012
Ion Ratio Lower Upper
50 100
52 30.4 23.0 42.8

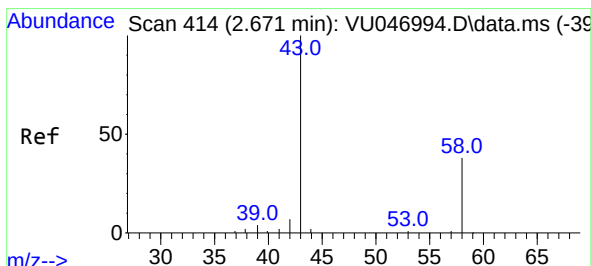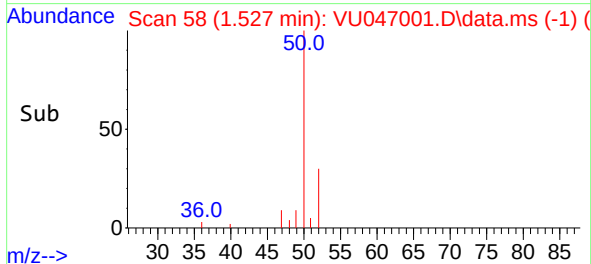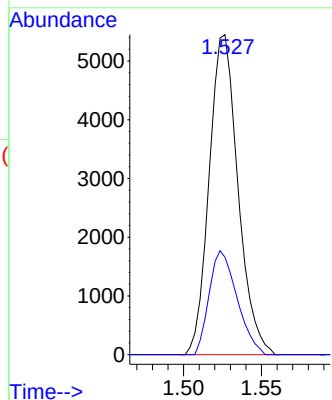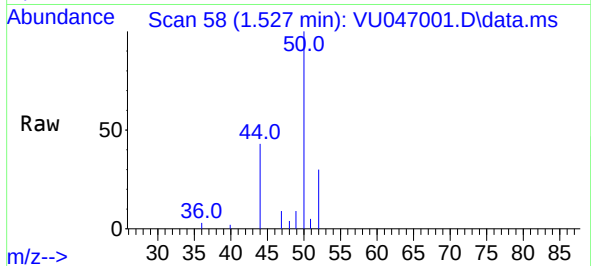

#13
Acetone
Concen: 4.100 ug/L
RT: 2.655 min Scan# 409
Delta R.T. -0.016 min
Lab File: VU047001.D
Acq: 02 Feb 2022 15:03

Tgt Ion: 43 Resp: 5503
Ion Ratio Lower Upper
43 100
58 35.1 0.0 71.6

