

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
 Data File : VU047009.D
 Acq On : 02 Feb 2022 18:16
 Operator : SY/MD
 Sample : VIBLK033
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK033

Quant Time: Feb 03 03:02:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 03 02:56:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	94449	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	111202	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	48162	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	44847	5.604	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	112.000%
7) Chloroethane-d5	1.919	69	35683	5.659	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.200%
11) 1,1-Dichloroethene-d2	2.572	65	16787	5.273	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	105.400%
20) 2-Butanone-d5	4.639	46	101465	42.795	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.580%
24) Chloroform-d	5.067	84	75059	5.342	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.800%
26) 1,2-Dichloroethane-d4	5.703	65	39724	5.192	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.800%
32) Benzene-d6	5.732	84	142136	4.349	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.000%
36) 1,2-Dichloropropane-d6	6.694	67	45843	4.672	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.400%
41) Toluene-d8	7.899	98	106410	3.557	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.200%
43) trans-1,3-Dichloroprop...	8.182	79	15451	3.585	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.800%
46) 2-Hexanone-d5	8.636	63	74488	29.192	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	58.380%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	38008	3.858	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	77.200%
66) 1,2-Dichlorobenzene-d4	12.195	152	38067	4.215	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.200%
Target Compounds						Qvalue
34) Trichloroethene	6.539	95	1314	0.193	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU047009.D
Acq On : 02 Feb 2022 18:16
Operator : SY/MD
Sample : VIBLK033
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK033


Quant Time: Feb 03 03:02:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 03 02:56:36 2022
Response via : Initial Calibration

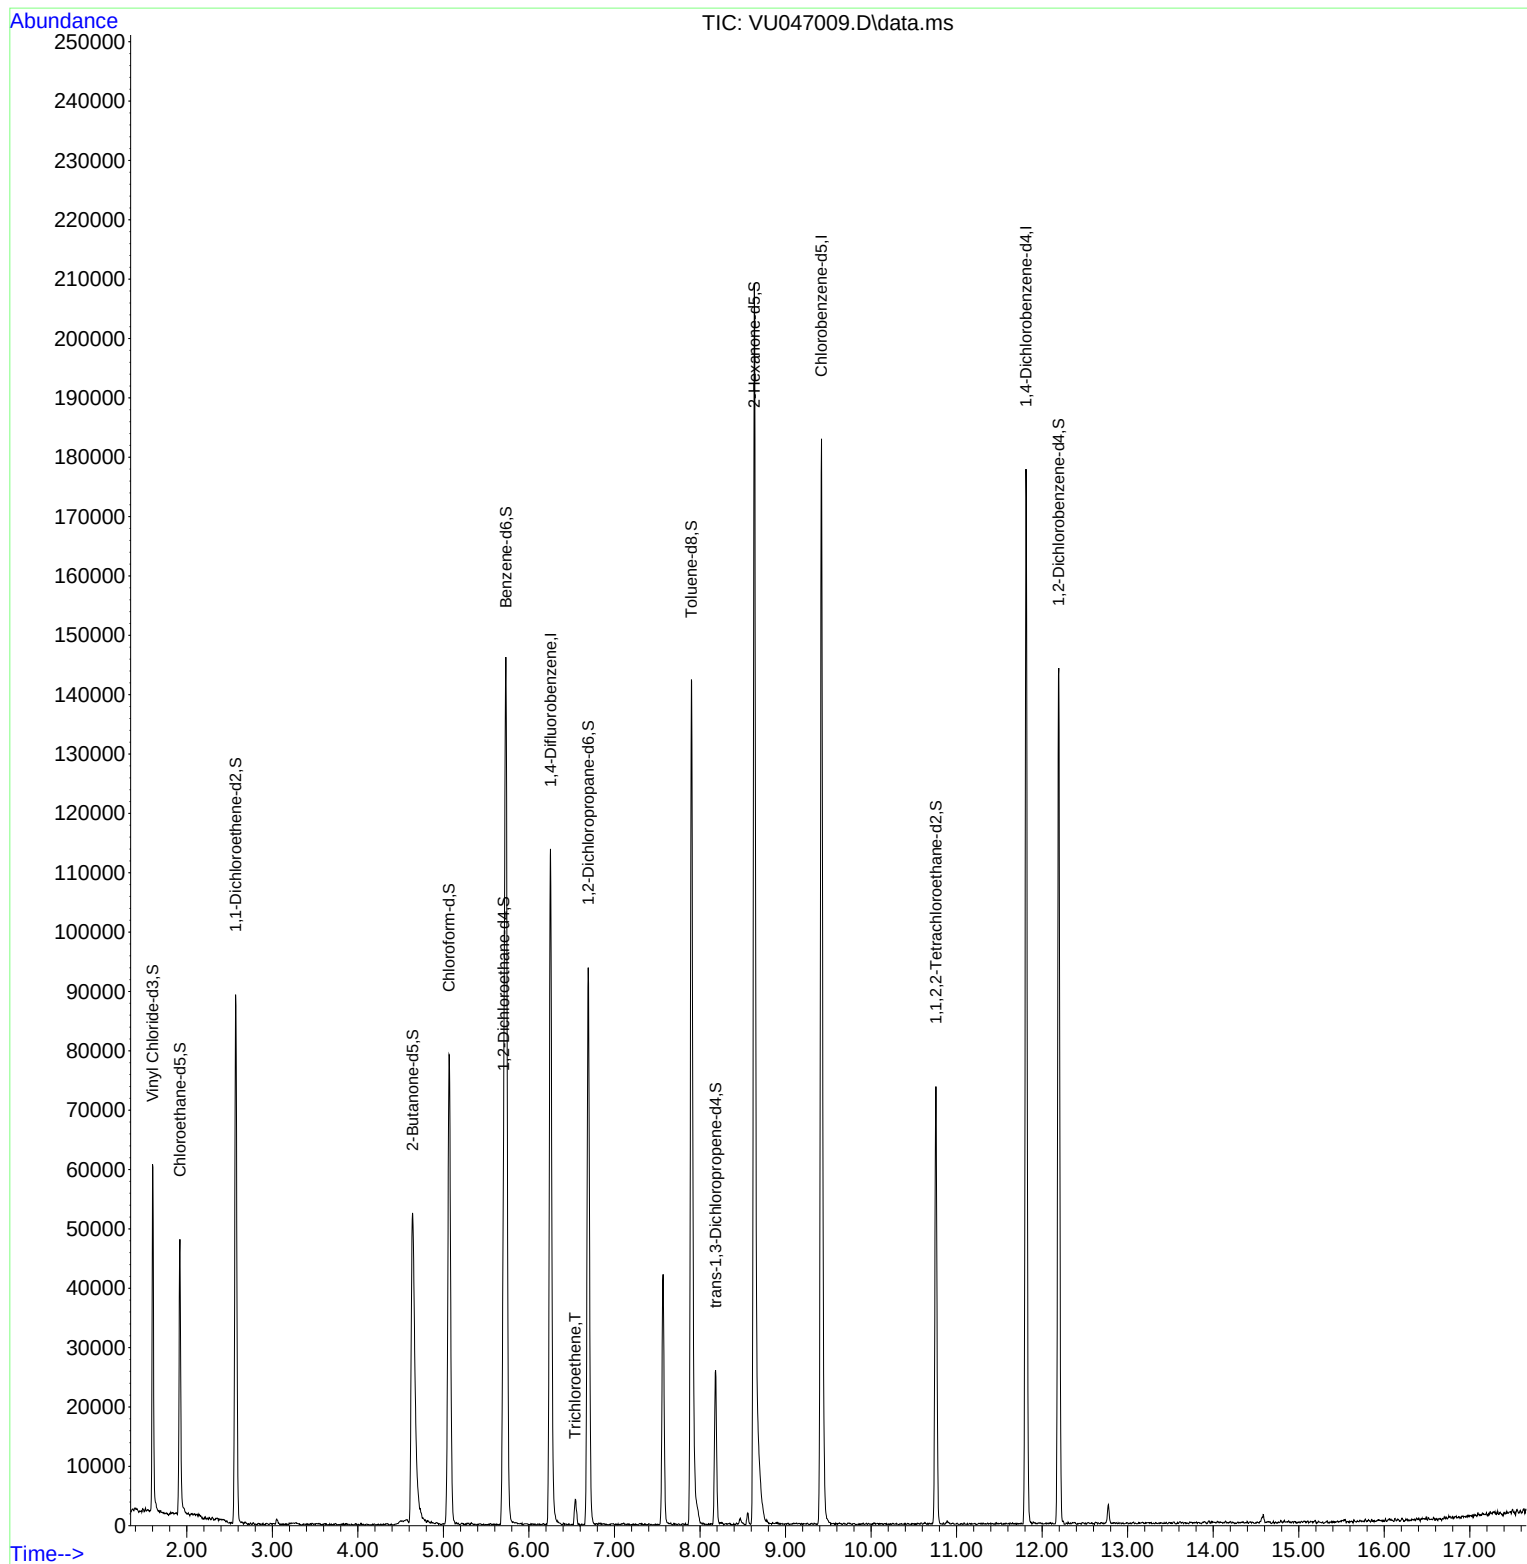

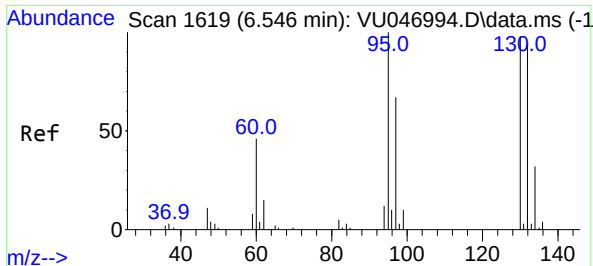

#34
 Trichloroethene
 Concen: 0.193 ug/L
 RT: 6.539 min Scan# 1
 Delta R.T. -0.007 min
 Lab File: VU047009.D
 Acq: 02 Feb 2022 18:16

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK033

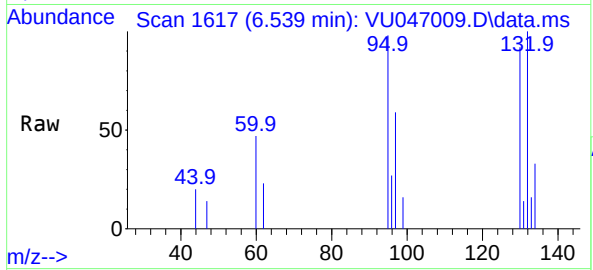

Tgt Ion: 95 Resp: 1314

Ion	Ratio	Lower	Upper
95	100		
97	59.6	46.5	86.5
132	101.8	65.1	120.9
130	93.5	67.3	124.9

