

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
 Data File : VU046998.D
 Acq On : 02 Feb 2022 13:51
 Operator : SY/MD
 Sample : N1349-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHP0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU046998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	14	rVB	7765	8262	1.85%	0.236%
2	1.527	50	58	68	rBV	7384	10514	2.35%	0.301%
3	1.604	74	82	97	rVB	61616	71003	15.87%	2.031%
4	1.919	171	180	200	rBV	49230	66398	14.84%	1.899%
5	2.575	371	384	401	rBV	90018	150347	33.61%	4.300%
6	3.051	518	532	546	rBV3	7812	15280	3.42%	0.437%
7	3.144	548	561	574	rBV2	26565	52330	11.70%	1.497%
8	4.636	1011	1025	1057	rBV2	64375	176191	39.39%	5.039%
9	4.813	1071	1080	1097	rVB2	6584	14833	3.32%	0.424%
10	5.070	1144	1160	1182	rBV	80510	189436	42.35%	5.418%
11	5.729	1345	1365	1389	rBV2	154922	404008	90.32%	11.555%
12	6.253	1513	1528	1555	rBV	125571	239041	53.44%	6.837%
13	6.694	1651	1665	1683	rBV	99058	191225	42.75%	5.469%
14	7.568	1925	1937	1954	rBV2	44786	78361	17.52%	2.241%
15	7.902	2026	2041	2059	rBV	156087	290694	64.99%	8.314%
16	8.182	2117	2128	2143	rBV	28725	48584	10.86%	1.390%
17	8.636	2256	2269	2309	rBV	237084	447312	100.00%	12.794%
18	9.420	2501	2513	2537	rBV	201049	347005	77.58%	9.925%
19	10.758	2916	2929	2947	rBV	81501	131145	29.32%	3.751%
20	11.812	3245	3257	3276	rVB	191509	304724	68.12%	8.716%
21	12.195	3365	3376	3393	rVB	162095	259617	58.04%	7.425%




Sum of corrected areas: 3496310

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU046998.D
Acq On : 02 Feb 2022 13:51
Operator : SY/MD
Sample : N1349-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

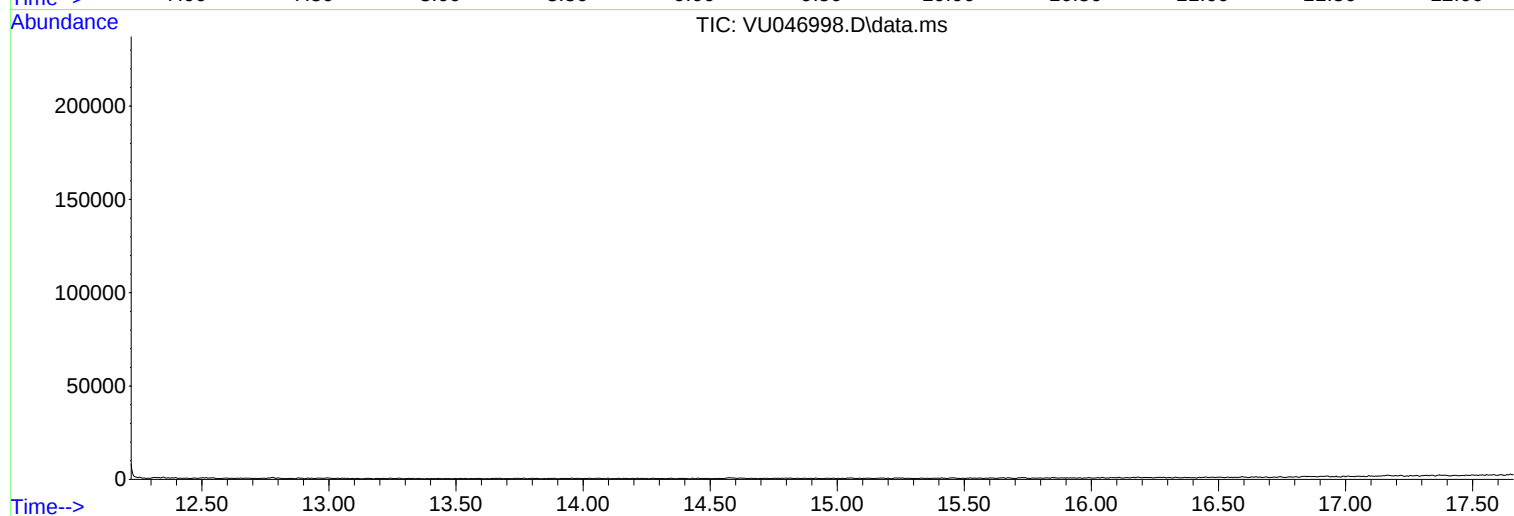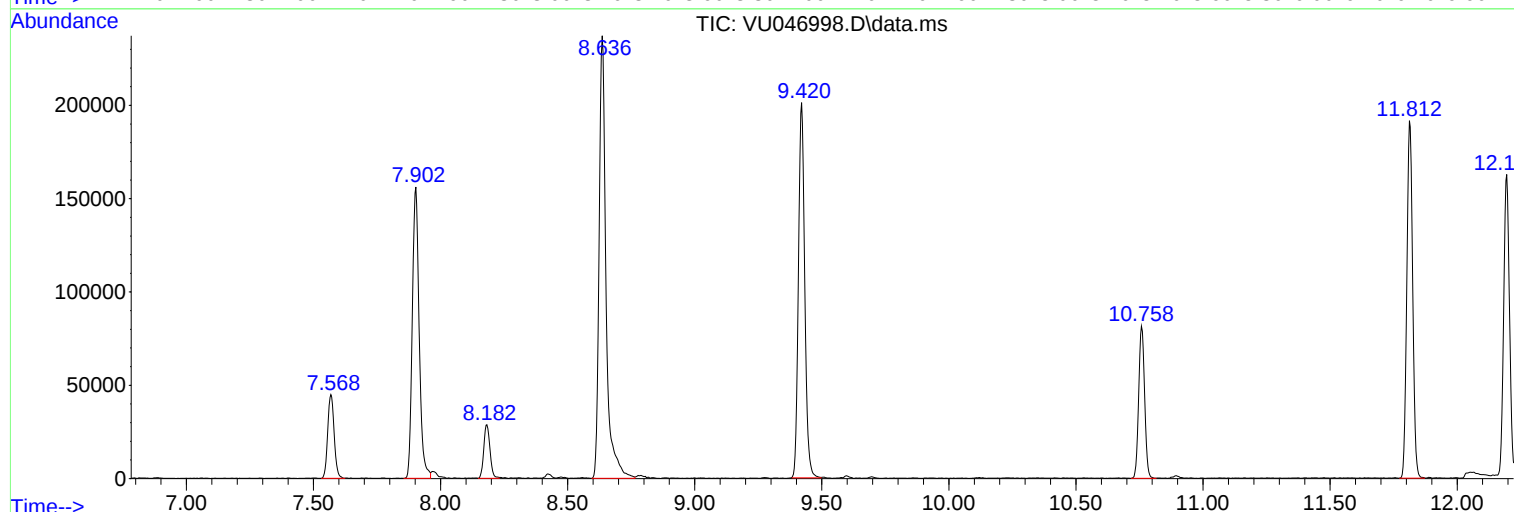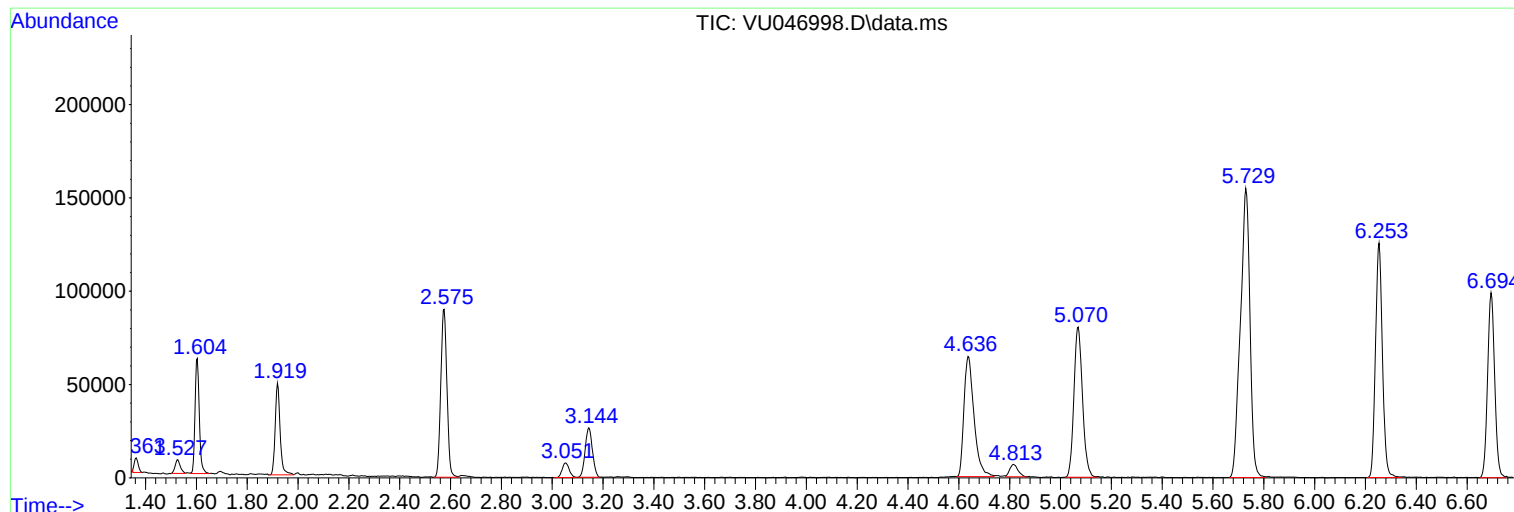

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU046998.D
Acq On : 02 Feb 2022 13:51
Operator : SY/MD
Sample : N1349-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHP0









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic3.144 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.144	1.09 ug/L	52330	1,4-Difluorobenzene	6.253

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Cyclobutane, methyl-	70	C5H10	000598-61-8	64
2		Cyclobutane, methyl-	70	C5H10	000598-61-8	64
3		Cyclopentane	70	C5H10	000287-92-3	64
4		1-Pentene	70	C5H10	000109-67-1	64
5		Cyclopentane	70	C5H10	000287-92-3	64

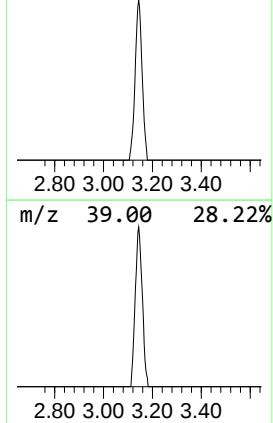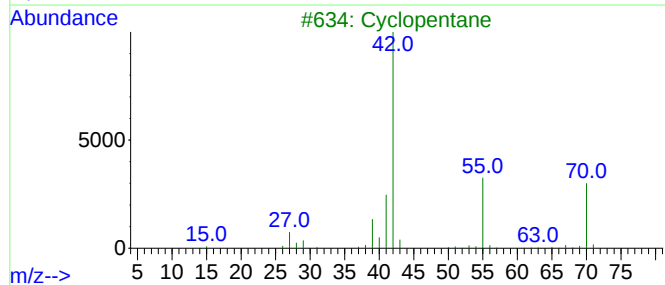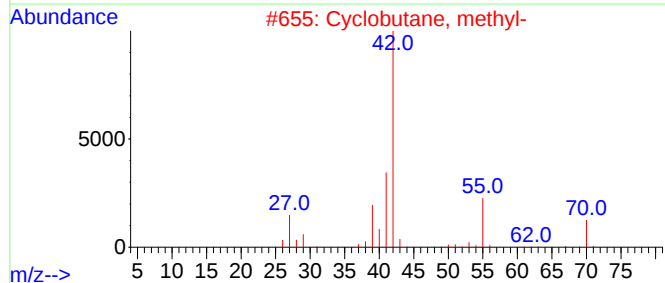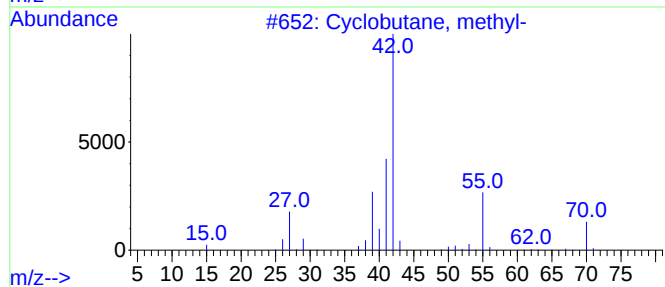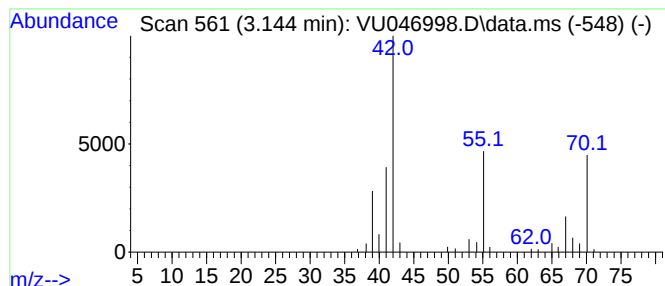

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU046998.D
Acq On : 02 Feb 2022 13:51
Operator : SY/MD
Sample : N1349-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	3.144	1.1	ug/L	52330	1	6.253	239041	5.0