

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
 Data File : VU047006.D
 Acq On : 02 Feb 2022 17:04
 Operator : SY/MD
 Sample : N1349-02 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HP1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	94	rBV	58161	65208	2.41%	0.950%
2	1.919	171	180	202	rBV	45331	62337	2.31%	0.908%
3	2.581	367	386	401	rBV4	166978	327655	12.12%	4.773%
4	4.636	1011	1025	1058	rBV2	59665	165696	6.13%	2.414%
5	5.067	1144	1159	1179	rBV2	77482	169070	6.26%	2.463%
6	5.321	1223	1238	1255	rBV	36053	79316	2.93%	1.155%
7	5.729	1345	1365	1385	rBV2	145033	379661	14.05%	5.531%
8	6.253	1515	1528	1548	rBV	113468	218072	8.07%	3.177%
9	6.546	1602	1619	1653	rBV	1455608	2702640	100.00%	39.370%
10	6.693	1653	1665	1682	rVB2	94740	188936	6.99%	2.752%
11	7.568	1926	1937	1954	rBV	43855	76384	2.83%	1.113%
12	7.902	2028	2041	2075	rBV	151360	287598	10.64%	4.189%
13	8.182	2117	2128	2144	rBV	27480	45236	1.67%	0.659%
14	8.555	2230	2244	2259	rBV	394482	692827	25.64%	10.092%
15	8.636	2259	2269	2310	rVB	230584	431816	15.98%	6.290%
16	9.420	2501	2513	2534	rBV	183324	325267	12.04%	4.738%
17	10.758	2917	2929	2943	rBV	75303	120604	4.46%	1.757%
18	11.812	3245	3257	3275	rBV	179239	286005	10.58%	4.166%
19	12.195	3364	3376	3392	rBV	148662	240470	8.90%	3.503%




Sum of corrected areas: 6864798

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU047006.D
Acq On : 02 Feb 2022 17:04
Operator : SY/MD
Sample : N1349-02 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

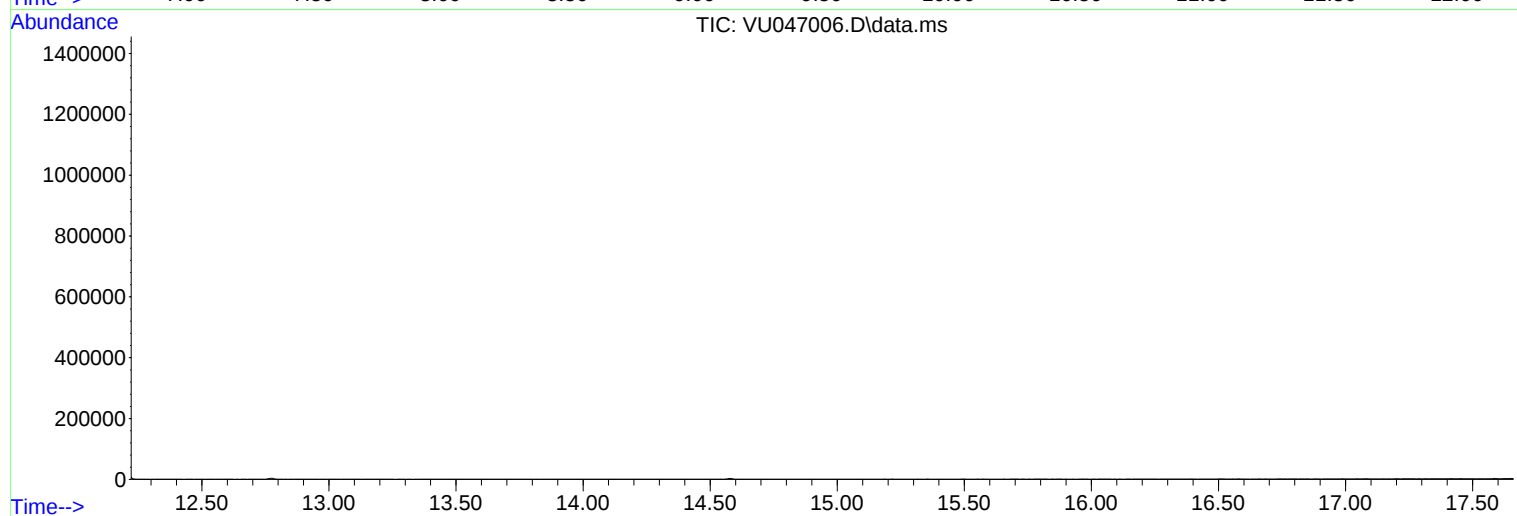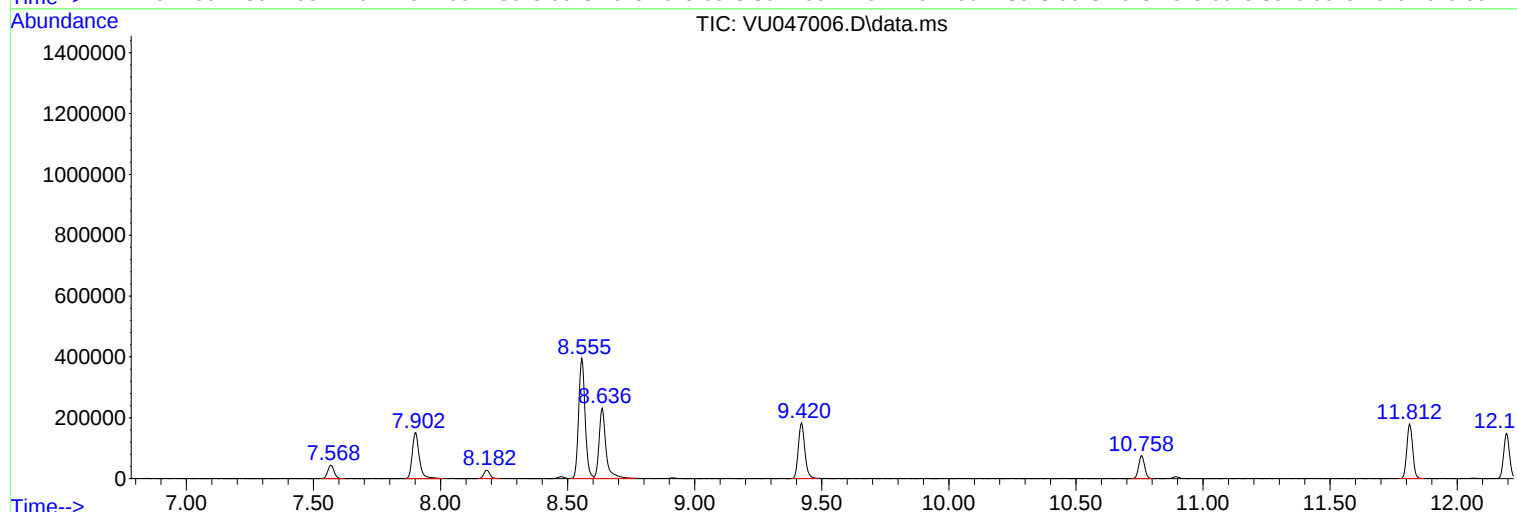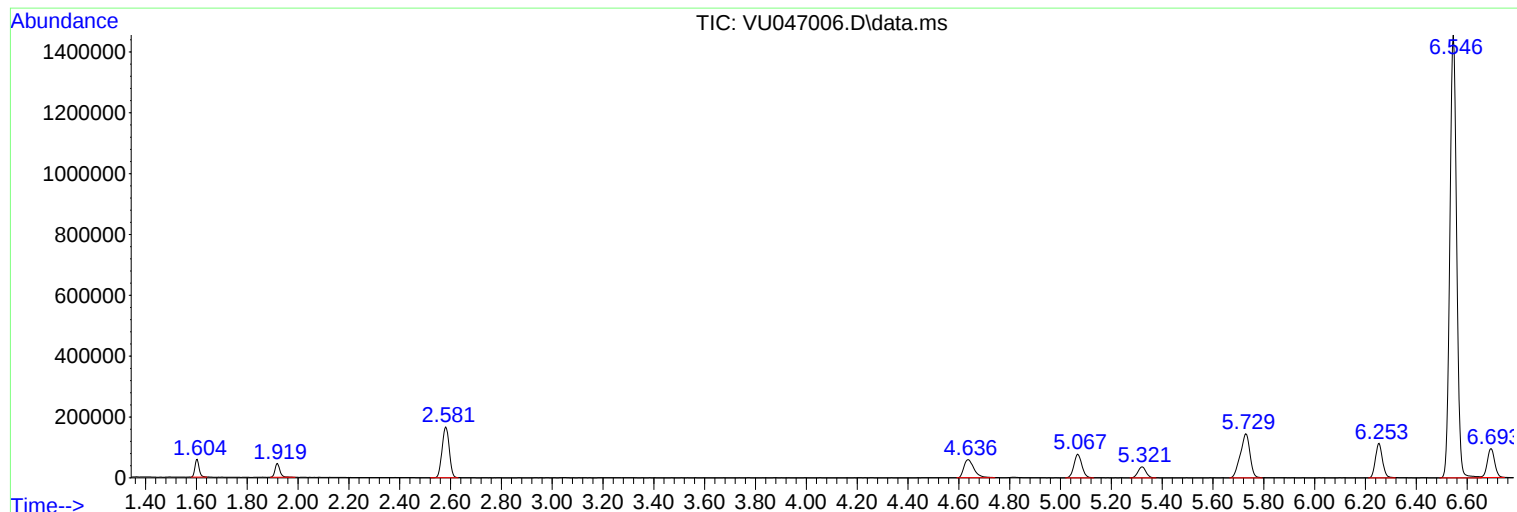

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU047006.D
Acq On : 02 Feb 2022 17:04
Operator : SY/MD
Sample : N1349-02 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU047006.D
Acq On : 02 Feb 2022 17:04
Operator : SY/MD
Sample : N1349-02 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
