

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
 Data File : VU047011.D
 Acq On : 02 Feb 2022 19:05
 Operator : SY/MD
 Sample : N1349-07 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HP6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	96	rBV	55793	65051	3.57%	1.116%
2	1.919	172	180	194	rBV	43734	59538	3.27%	1.021%
3	2.578	372	385	404	rBV3	129750	252654	13.86%	4.333%
4	4.668	1012	1035	1064	rBV2	139625	429361	23.55%	7.363%
5	4.819	1069	1082	1098	rVV3	8893	20529	1.13%	0.352%
6	5.067	1143	1159	1180	rBV	76141	169247	9.28%	2.902%
7	5.321	1222	1238	1253	rBV2	21642	48482	2.66%	0.831%
8	5.729	1344	1365	1387	rBV2	145287	379120	20.80%	6.501%
9	6.253	1514	1528	1552	rBV	116274	221323	12.14%	3.795%
10	6.546	1604	1619	1640	rBV	206725	384790	21.11%	6.599%
11	6.693	1650	1665	1685	rBV2	93223	181780	9.97%	3.117%
12	7.568	1925	1937	1956	rBV	40653	71722	3.93%	1.230%
13	7.902	2028	2041	2060	rBV	143414	269707	14.80%	4.625%
14	8.182	2117	2128	2143	rBV	26237	43436	2.38%	0.745%
15	8.555	2230	2244	2259	rBV	1048844	1822877	100.00%	31.260%
16	8.635	2259	2269	2313	rVB	229047	444597	24.39%	7.624%
17	9.420	2500	2513	2533	rBV	184576	329290	18.06%	5.647%
18	10.758	2918	2929	2945	rVB	74269	119705	6.57%	2.053%
19	11.812	3245	3257	3275	rBV	176600	284161	15.59%	4.873%
20	12.195	3360	3376	3392	rBV2	144882	234026	12.84%	4.013%




Sum of corrected areas: 5831396

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU047011.D
Acq On : 02 Feb 2022 19:05
Operator : SY/MD
Sample : N1349-07 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

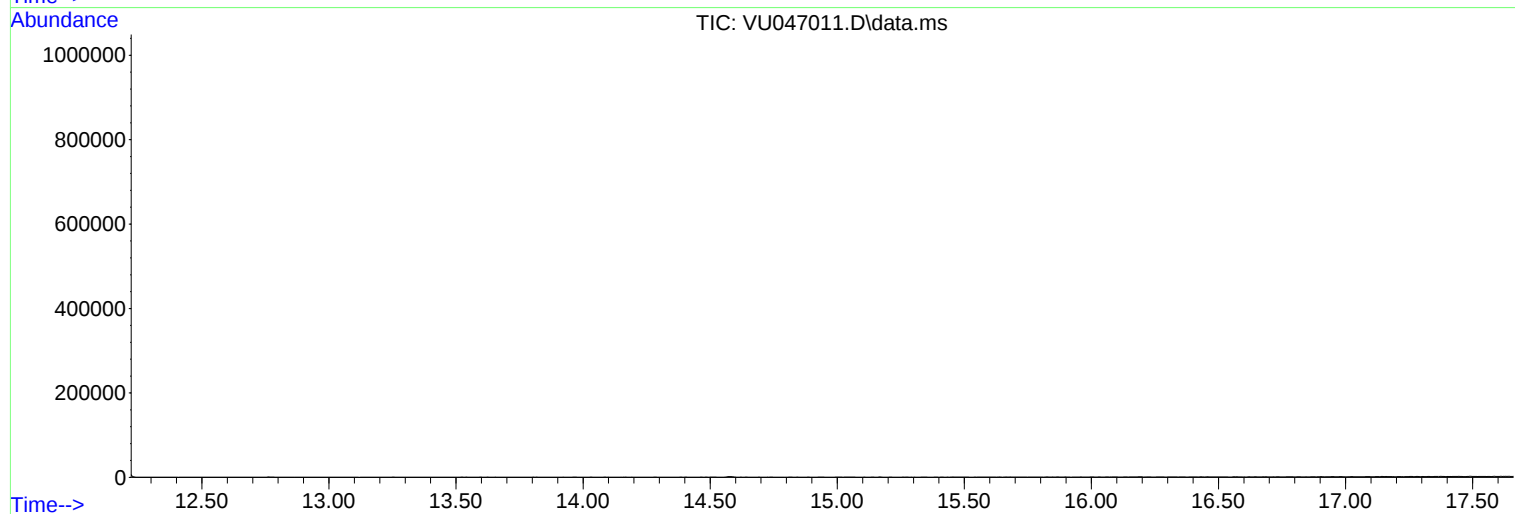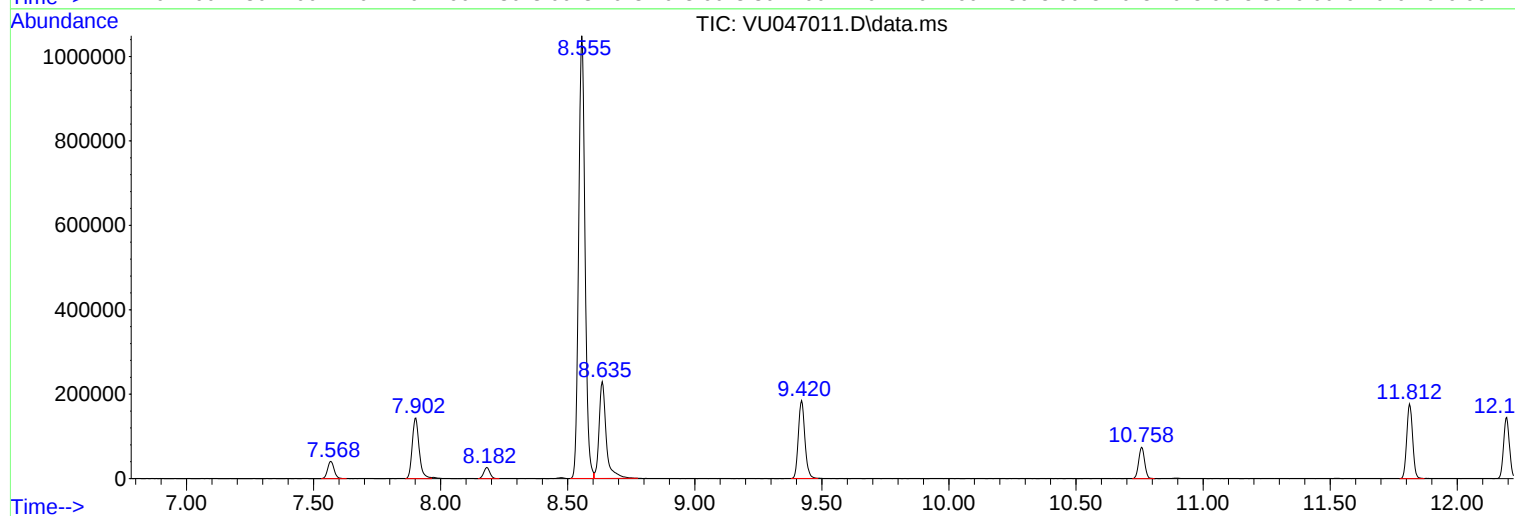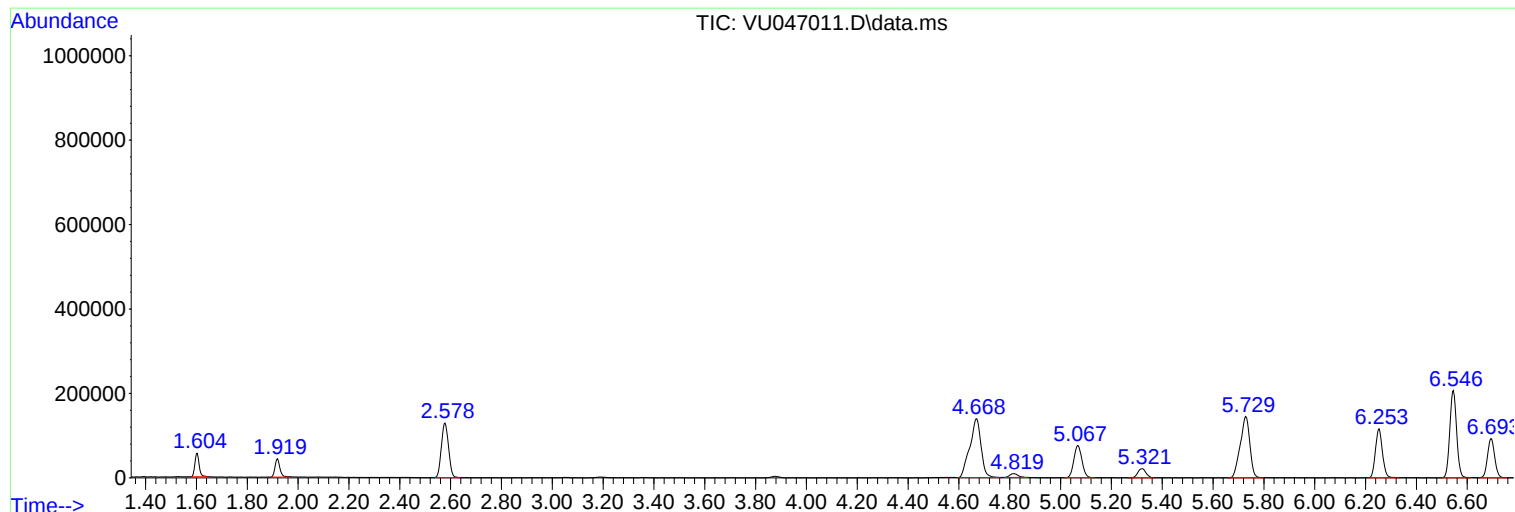

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU047011.D
Acq On : 02 Feb 2022 19:05
Operator : SY/MD
Sample : N1349-07 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
Data File : VU047011.D
Acq On : 02 Feb 2022 19:05
Operator : SY/MD
Sample : N1349-07 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc