


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020222\
 Data File : VU046993.D
 Acq On : 02 Feb 2022 10:12
 Operator : SY/MD
 Sample : BFB052
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB052

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Feb 03 02:56:36 2022

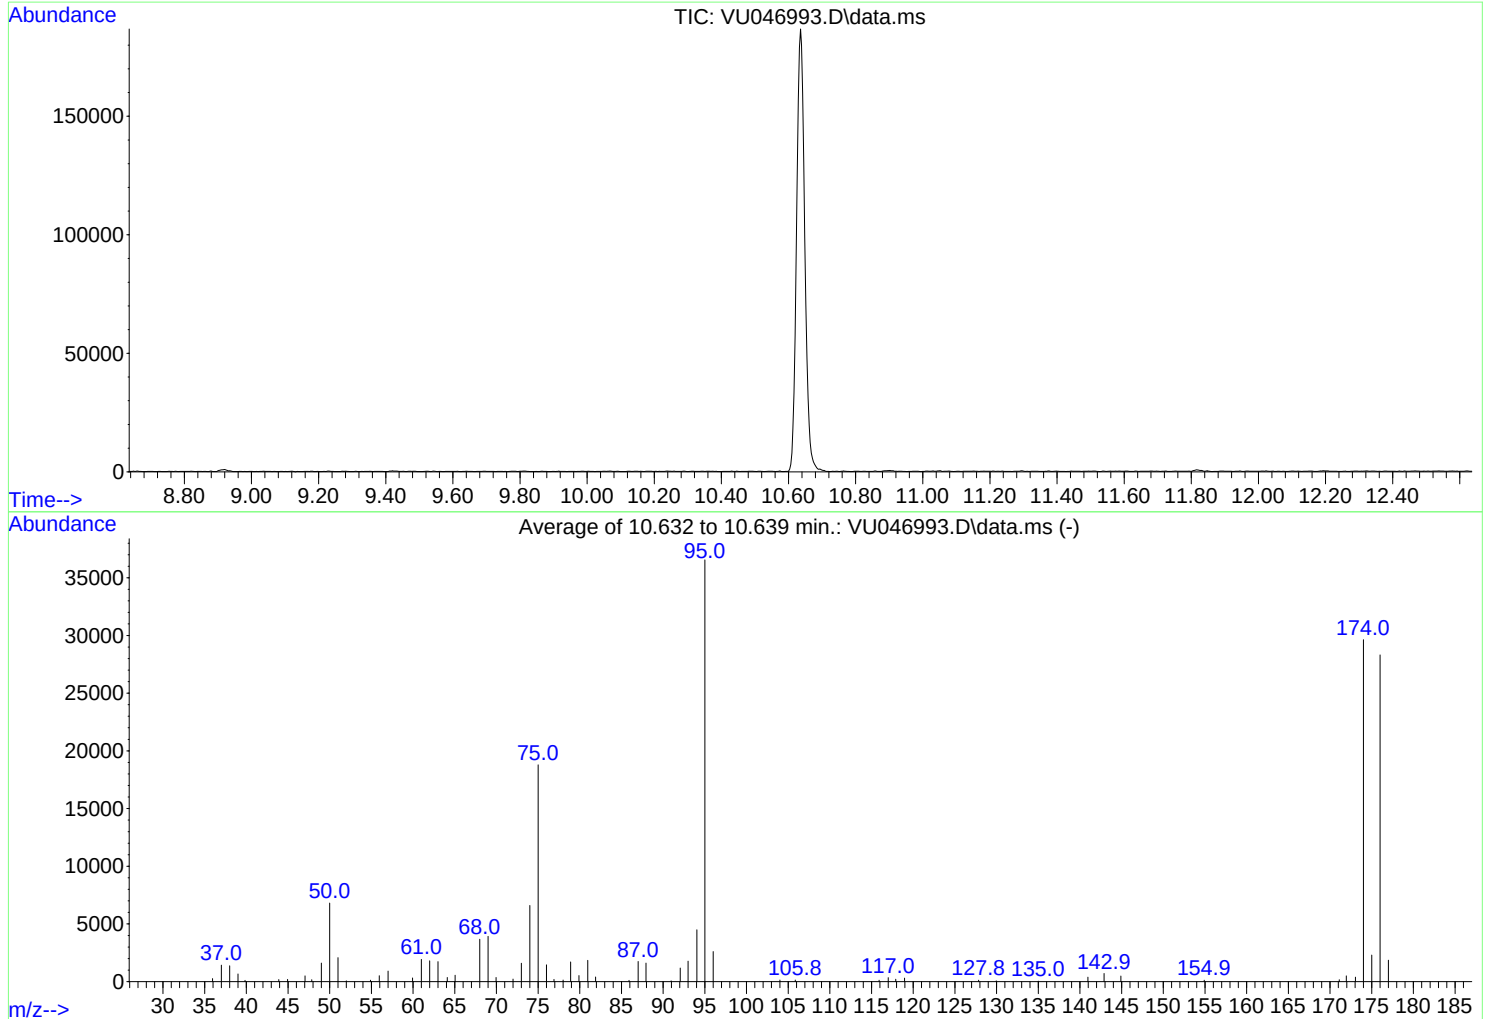

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	6804	PASS
75	95	30	80	51.4	18784	PASS
95	95	100	100	100.0	36555	PASS
96	95	5	9	7.1	2606	PASS
173	174	0.00	2	1.3	386	PASS
174	95	50	120	81.1	29632	PASS
175	174	5	9	7.8	2299	PASS
176	174	95	101	95.5	28312	PASS
177	176	5	9	6.6	1858	PASS

m/z	Abundance
43.90	196.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

m/z	Abundance
36.00	243.0
37.00	1449.0
38.00	1356.0
39.00	651.0
39.80	113.0
43.90	325.0
45.00	194.0
47.10	457.0
47.80	175.0
49.00	1522.0
50.00	6797.0
51.00	1927.0
52.00	114.0
54.90	133.0
55.90	504.0
57.00	925.0
60.00	332.0
61.00	1853.0
62.00	1734.0
63.00	1685.0
64.10	341.0
65.10	532.0
68.00	3653.0
69.00	3886.0
70.00	325.0
72.00	195.0
73.00	1666.0
74.00	6512.0
75.00	18816.0
76.00	1471.0
76.90	182.0
78.00	158.0
78.90	1731.0
79.90	488.0
81.00	1840.0
81.90	372.0
85.90	108.0
87.00	1779.0
87.90	1608.0
91.00	119.0
92.10	1091.0
93.00	1743.0
94.00	4436.0
95.00	36704.0
96.00	2616.0
104.00	134.0
105.80	159.0
115.90	121.0
117.00	354.0
117.90	190.0
119.00	281.0
127.90	116.0
141.00	351.0
142.90	710.0
144.90	414.0
154.90	139.0
171.10	161.0
171.90	485.0
173.00	422.0
174.00	28128.0
175.00	2430.0
176.00	27544.0
177.00	1916.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

m/z	Abundance
35.90	269.0
37.00	1441.0
38.00	1387.0
39.00	672.0
39.90	107.0
44.00	378.0
44.90	194.0
47.10	546.0
47.80	174.0
49.00	1680.0
50.00	7065.0
51.00	2136.0
52.00	105.0
54.90	130.0
56.00	525.0
57.00	955.0
60.00	306.0
61.00	1988.0
62.00	1842.0
63.00	1785.0
64.10	366.0
65.00	568.0
68.00	3776.0
69.00	4034.0
69.90	382.0
72.00	222.0
73.00	1646.0
74.00	6820.0
75.00	19264.0
76.00	1509.0
76.90	205.0
78.00	129.0
78.90	1773.0
79.90	536.0
81.00	1901.0
81.90	405.0
85.90	124.0
87.00	1775.0
88.00	1675.0
90.90	102.0
92.00	1195.0
93.00	1856.0
94.10	4596.0
95.00	37408.0
96.00	2713.0
104.00	151.0
105.90	140.0
115.90	117.0
117.00	351.0
117.90	233.0
118.90	329.0
127.90	122.0
130.00	106.0
140.90	411.0
142.90	724.0
144.90	518.0
154.90	128.0
171.10	177.0
172.00	508.0
173.10	390.0
174.00	30336.0
175.00	2308.0
176.00	29144.0
177.00	1896.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

m/z	Abundance
35.90	265.0
37.00	1382.0
38.00	1380.0
39.00	667.0
39.90	123.0
43.90	411.0
44.90	190.0
47.00	492.0
47.90	157.0
49.00	1619.0
50.00	6550.0
51.00	2162.0
54.90	118.0
55.90	530.0
57.00	888.0
59.90	322.0
61.00	1953.0
62.00	1827.0
63.00	1732.0
64.10	379.0
65.00	551.0
68.00	3601.0
69.00	3873.0
69.90	389.0
72.00	254.0
73.00	1481.0
74.00	6461.0
75.00	18272.0
76.00	1410.0
76.90	215.0
78.00	118.0
78.90	1634.0
79.90	569.0
80.90	1783.0
81.90	419.0
85.90	116.0
87.00	1701.0
88.00	1549.0
92.00	1258.0
93.00	1716.0
94.10	4452.0
95.00	35552.0
96.00	2488.0
104.00	140.0
105.90	139.0
115.90	124.0
117.00	355.0
117.90	207.0
119.00	328.0
127.80	123.0
129.90	102.0
135.00	118.0
140.90	420.0
142.90	683.0
144.90	511.0
154.90	128.0
171.10	151.0
172.00	512.0
173.00	346.0
174.00	30432.0
175.00	2158.0
176.00	28248.0
177.00	1762.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052