


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU020722\
 Data File : VU047058.D
 Acq On : 07 Feb 2022 08:57
 Operator : SY/MD
 Sample : BFB055
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB055

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR020422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Feb 07 22:28:35 2022

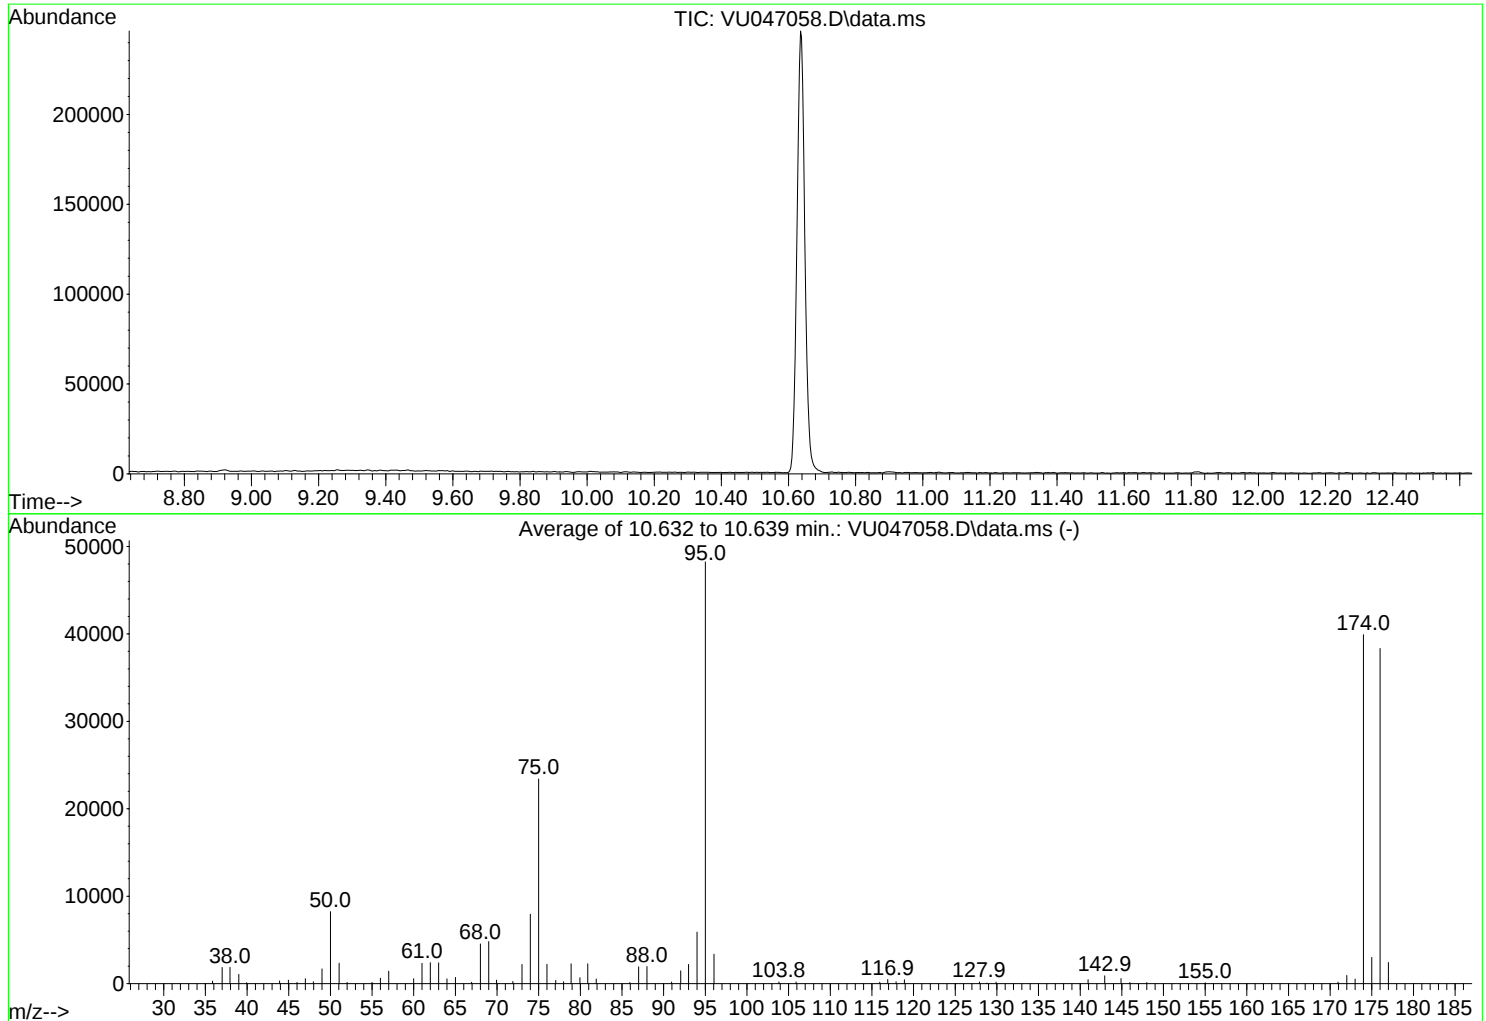

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	8228	PASS
75	95	30	80	48.5	23413	PASS
95	95	100	100	100.0	48240	PASS
96	95	5	9	7.0	3371	PASS
173	174	0.00	2	1.4	541	PASS
174	95	50	120	82.7	39907	PASS
175	174	5	9	7.5	3004	PASS
176	174	95	101	96.1	38347	PASS
177	176	5	9	6.3	2416	PASS

m/z	Abundance
35.90	391.0
37.90	128.0
43.90	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055

m/z	Abundance
35.90	696.0
37.00	1701.0
38.00	1946.0
39.00	1032.0
39.90	103.0
43.90	442.0
45.00	349.0
46.00	150.0
47.00	504.0
47.90	187.0
49.00	1577.0
50.00	8110.0
51.10	2347.0
52.00	110.0
55.00	147.0
56.00	589.0
57.00	1366.0
60.00	572.0
61.00	2302.0
62.00	2237.0
63.00	2225.0
64.00	606.0
65.00	674.0
66.90	201.0
68.00	4460.0
69.00	4562.0
69.90	411.0
71.90	236.0
73.00	2130.0
74.00	7809.0
75.00	22736.0
76.00	2139.0
77.00	336.0
77.90	153.0
78.90	2224.0
80.00	604.0
80.90	2183.0
81.90	466.0
85.90	106.0
87.00	1926.0
88.00	1779.0
91.00	197.0
92.00	1490.0
93.00	2103.0
94.00	5673.0
95.00	45904.0
96.00	3253.0
103.80	164.0
105.90	166.0
115.90	161.0
116.90	483.0
117.90	207.0
118.90	420.0
127.90	175.0
129.90	193.0
141.00	411.0
142.90	855.0
144.90	537.0
145.90	111.0
148.00	116.0
155.00	105.0
171.00	150.0
172.00	892.0
173.00	558.0
174.00	36664.0
175.00	2886.0
176.00	35616.0
177.00	2360.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055

m/z	Abundance
35.90	680.0
37.00	1926.0
38.00	2036.0
39.00	1102.0
40.00	102.0
43.90	492.0
44.90	438.0
46.00	161.0
47.00	586.0
47.90	221.0
49.00	1726.0
50.00	8456.0
51.10	2428.0
52.00	149.0
55.00	171.0
56.00	646.0
57.00	1513.0
60.00	602.0
61.00	2402.0
62.00	2472.0
63.00	2539.0
64.00	577.0
65.00	738.0
66.90	167.0
68.00	4728.0
69.00	4919.0
69.90	425.0
71.90	283.0
73.00	2302.0
74.00	8146.0
75.00	24192.0
76.00	2275.0
77.10	366.0
78.00	229.0
78.90	2381.0
80.00	688.0
80.90	2276.0
81.90	526.0
86.00	133.0
87.00	1933.0
88.00	2012.0
90.90	188.0
92.10	1484.0
93.00	2251.0
94.00	6133.0
95.00	49968.0
96.00	3479.0
103.90	209.0
105.90	204.0
116.00	170.0
116.90	512.0
117.90	221.0
118.90	447.0
127.90	201.0
128.80	111.0
129.90	194.0
140.90	465.0
143.00	905.0
144.90	631.0
146.00	128.0
148.00	143.0
155.00	106.0
170.90	170.0
172.00	987.0
173.00	562.0
174.00	41296.0
175.00	3088.0
176.00	39576.0
177.00	2437.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055

m/z	Abundance
35.90	674.0
37.00	1938.0
38.00	1994.0
39.00	1050.0
40.00	134.0
43.90	497.0
44.90	444.0
46.00	137.0
47.00	607.0
48.00	240.0
49.00	1753.0
50.00	8119.0
51.00	2281.0
52.00	162.0
55.00	148.0
56.00	640.0
57.00	1409.0
60.00	529.0
61.00	2273.0
62.00	2493.0
63.00	2378.0
64.00	491.0
65.00	742.0
67.00	131.0
68.00	4444.0
69.00	4963.0
70.00	398.0
71.90	261.0
73.00	2145.0
74.00	7889.0
75.00	23312.0
76.00	2215.0
77.10	381.0
78.10	261.0
78.90	2233.0
79.90	717.0
80.90	2328.0
81.90	579.0
86.00	125.0
87.00	1904.0
88.00	2101.0
90.90	159.0
92.10	1402.0
93.00	2232.0
94.00	5892.0
95.00	48848.0
96.10	3380.0
103.90	232.0
105.90	228.0
116.00	187.0
116.90	456.0
117.90	241.0
118.90	433.0
127.90	203.0
128.80	102.0
129.90	192.0
140.90	485.0
143.00	921.0
144.90	612.0
146.00	137.0
148.00	149.0
155.00	114.0
170.90	229.0
172.00	940.0
173.00	504.0
174.00	41760.0
175.00	3037.0
176.00	39848.0
177.00	2452.0

Instrument :
MSVOA_U
ClientSampleId :
BFB055