

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047119.D
 Acq On : 11 Feb 2022 16:46
 Operator : SY/MD
 Sample : N1474-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Feb 12 01:29:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Feb 12 01:25:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	442647	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	411806	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	211839	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	174157	43.321	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.640%		
7) Chloroethane-d5	1.919	69	142659	47.870	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	95.740%		
11) 1,1-Dichloroethene-d2	2.575	63	232072	34.835	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.680%		
21) 2-Butanone-d5	4.629	46	354091	113.569	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	113.570%		
24) Chloroform-d	5.067	84	301587	46.210	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.420%		
26) 1,2-Dichloroethane-d4	5.703	65	204640	48.852	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.700%		
32) Benzene-d6	5.729	84	647726	47.311	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.620%		
36) 1,2-Dichloropropane-d6	6.694	67	215168	48.463	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.920%		
41) Toluene-d8	7.899	98	610048	46.800	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.600%		
43) trans-1,3-Dichloroprop...	8.179	79	107432	46.174	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.340%		
47) 2-Hexanone-d5	8.632	63	263782	103.706	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	103.710%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	310672	47.989	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.980%		
66) 1,2-Dichlorobenzene-d4	12.195	152	237938	47.359	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.720%		
Target Compounds						Qvalue
20) cis-1,2-Dichloroethene	4.674	96	3667	1.096	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047119.D
Acq On : 11 Feb 2022 16:46
Operator : SY/MD
Sample : N1474-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Feb 12 01:29:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 12 01:25:35 2022
Response via : Initial Calibration

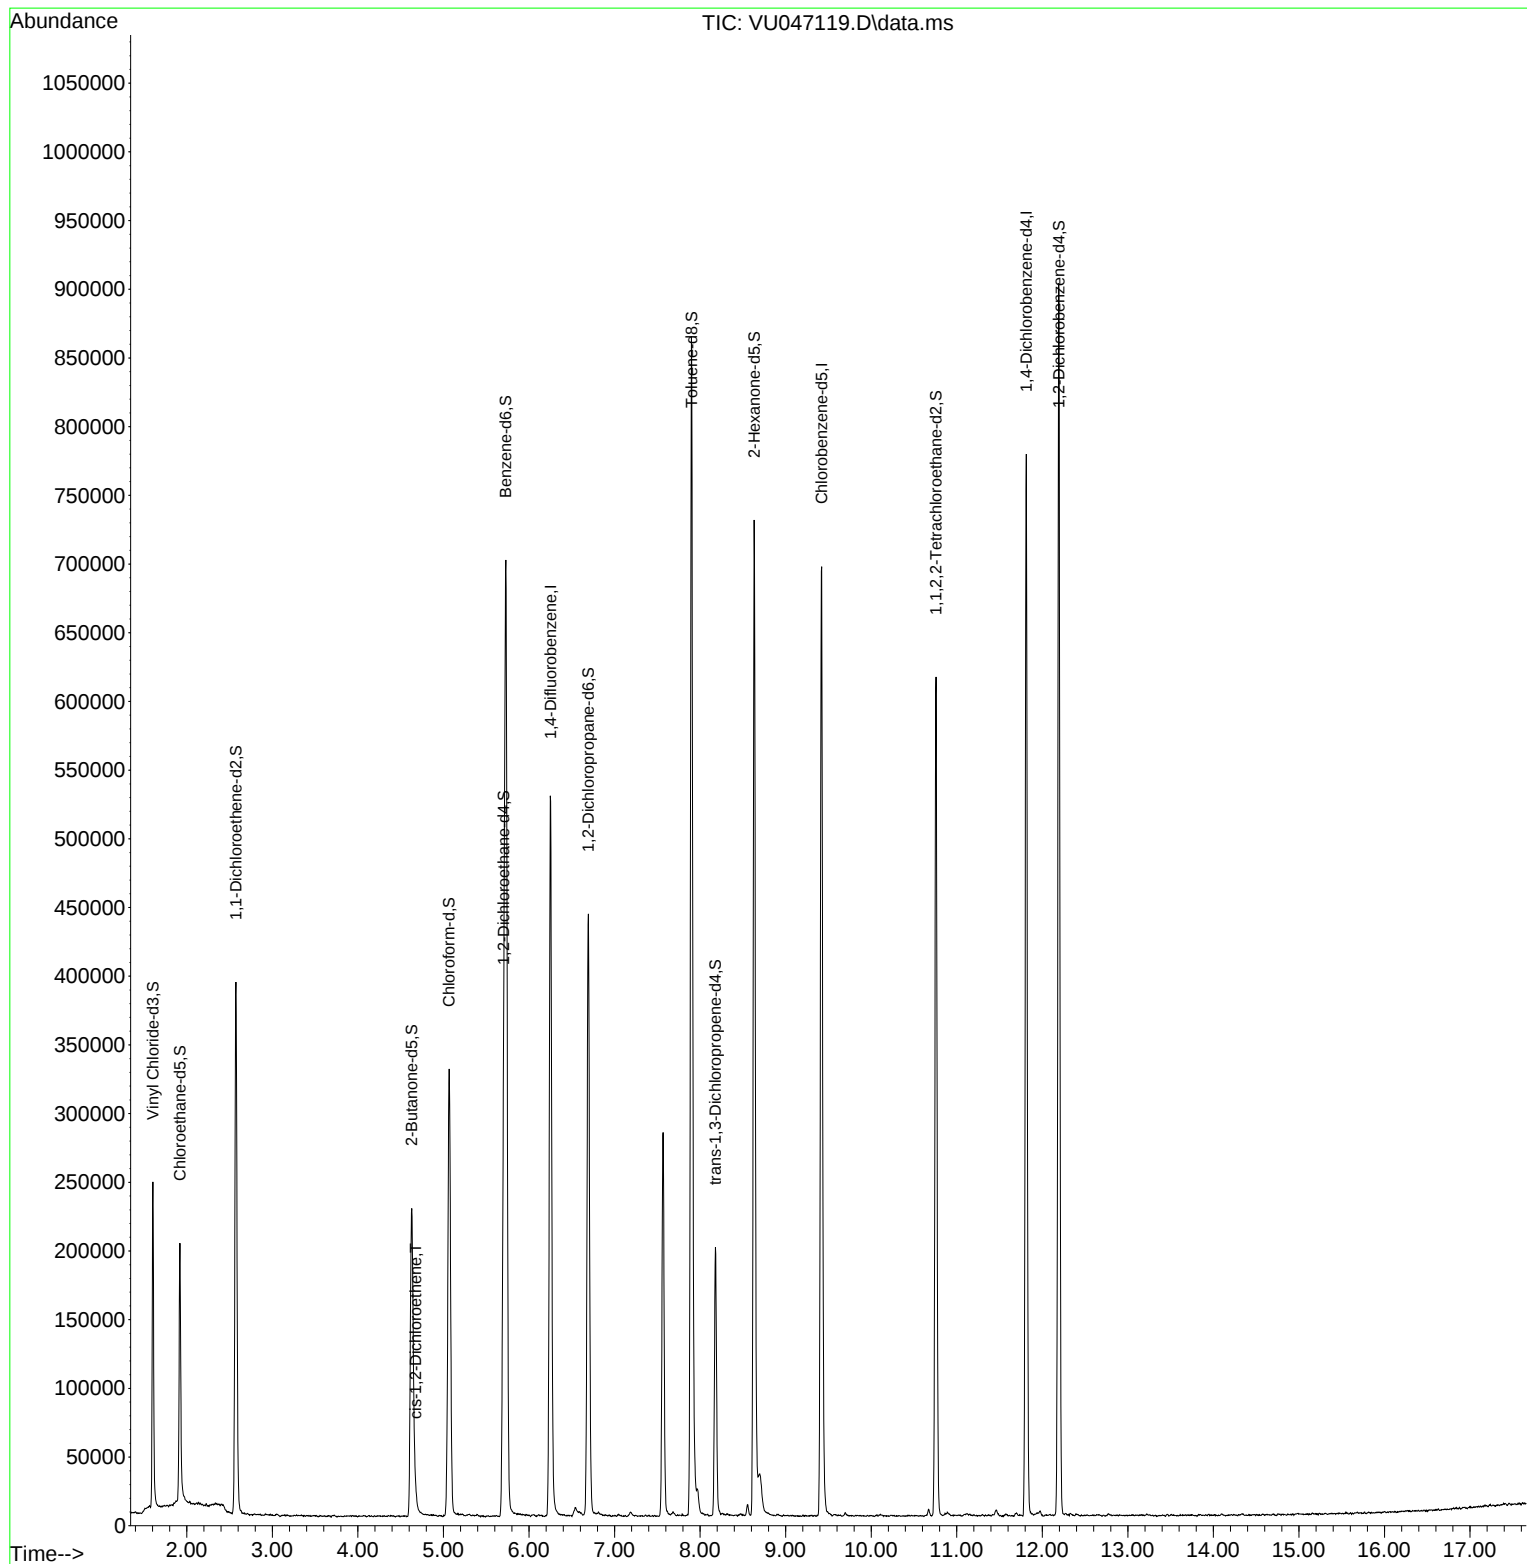

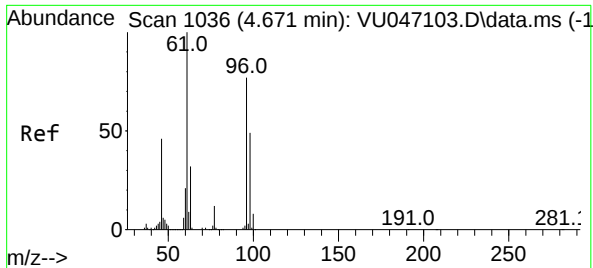

#20
 cis-1,2-Dichloroethene
 Concen: 1.096 ug/L
 RT: 4.674 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VU047119.D
 Acq: 11 Feb 2022 16:46

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Tgt Ion:	96	Resp:	3667
Ion	Ratio	Lower	Upper
96	100		
61	105.6	86.0	159.6
68	0.0	0.0	0.0

