

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047113.D
 Acq On : 11 Feb 2022 14:31
 Operator : SY/MD
 Sample : N1462-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	101	rVB	237708	277096	14.10%	1.651%
2	1.919	174	180	202	rVB	189126	255430	12.99%	1.522%
3	2.575	373	384	401	rBV	395853	662194	33.69%	3.946%
4	3.031	524	526	528	rVB3	863	341	0.02%	0.002%
5	3.057	529	534	538	rBV6	1389	1671	0.09%	0.010%
6	3.179	569	572	578	rVB8	1204	1024	0.05%	0.006%
7	3.282	601	604	605	rBV3	643	342	0.02%	0.002%
8	3.494	667	670	675	rBV7	1307	1310	0.07%	0.008%
9	3.597	699	702	705	rBV3	1206	944	0.05%	0.006%
10	3.681	724	728	729	rBV4	648	404	0.02%	0.002%
11	3.716	736	739	745	rVB8	1147	1146	0.06%	0.007%
12	3.761	748	753	756	rBV6	656	511	0.03%	0.003%
13	3.825	765	773	774	rBV8	912	927	0.05%	0.006%
14	3.883	788	791	792	rBV	367	171	0.01%	0.001%
15	3.896	792	795	798	rVV4	729	486	0.02%	0.003%
16	3.948	807	811	813	rBV4	534	411	0.02%	0.002%
17	3.980	817	821	823	rBV4	1256	807	0.04%	0.005%
18	4.018	829	833	837	rBV6	1114	1132	0.06%	0.007%
19	4.038	837	839	840	rVV2	455	143	0.01%	0.001%
20	4.047	840	842	844	rVB2	297	135	0.01%	0.001%
21	4.067	846	848	852	rBV4	674	452	0.02%	0.003%
22	4.141	869	871	874	rBV3	499	236	0.01%	0.001%
23	4.157	874	876	878	rVV3	356	136	0.01%	0.001%
24	4.195	885	888	890	rBV3	608	422	0.02%	0.003%
25	4.279	907	914	917	rBV8	716	1046	0.05%	0.006%
26	4.305	920	922	925	rVV4	852	661	0.03%	0.004%
27	4.337	929	932	935	rBV4	938	756	0.04%	0.005%
28	4.353	935	937	939	rBV2	347	145	0.01%	0.001%
29	4.366	939	941	944	rBV4	719	402	0.02%	0.002%
30	4.398	950	951	955	rVB4	521	230	0.01%	0.001%
31	4.417	955	957	958	rBV2	452	135	0.01%	0.001%
32	4.440	961	964	968	rVB6	701	568	0.03%	0.003%
33	4.469	968	973	977	rBV6	1062	1022	0.05%	0.006%
34	4.559	997	1001	1005	rBV4	606	666	0.03%	0.004%
35	4.629	1008	1023	1061	rBV	243466	762549	38.79%	4.544%
36	5.002	1137	1139	1140	rBV2	650	289	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047113.D
 Acq On : 11 Feb 2022 14:31
 Operator : SY/MD
 Sample : N1462-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	5.067	1145	1159	1177	rVV	341424	745223	37.91%	4.441%
38	5.456	1276	1280	1283	rVB6	634	604	0.03%	0.004%
39	5.478	1285	1287	1291	rVB3	798	460	0.02%	0.003%
40	5.507	1293	1296	1298	rBV4	728	506	0.03%	0.003%
41	5.549	1307	1309	1312	rVB3	681	287	0.01%	0.002%
42	5.575	1312	1317	1318	rBV4	596	503	0.03%	0.003%
43	5.613	1327	1329	1330	rVB2	424	108	0.01%	0.001%
44	5.632	1330	1335	1337	rBV5	570	554	0.03%	0.003%
45	5.729	1342	1365	1391	rBV2	721823	1965671	100.00%	11.713%
46	6.253	1514	1528	1553	rBV	551692	1064766	54.17%	6.345%
47	6.407	1573	1576	1578	rBV4	1263	929	0.05%	0.006%
48	6.546	1606	1619	1635	rBV2	47040	99079	5.04%	0.590%
49	6.694	1652	1665	1687	rVB	456439	883265	44.93%	5.263%
50	6.954	1744	1746	1748	rBV3	531	202	0.01%	0.001%
51	7.005	1758	1762	1767	rBV6	1047	1033	0.05%	0.006%
52	7.134	1798	1802	1805	rBV5	936	774	0.04%	0.005%
53	7.160	1805	1810	1812	rBV4	1138	937	0.05%	0.006%
54	7.256	1838	1840	1844	rBV5	455	365	0.02%	0.002%
55	7.321	1855	1860	1861	rBV4	613	543	0.03%	0.003%
56	7.378	1876	1878	1879	rBV2	378	175	0.01%	0.001%
57	7.433	1890	1895	1896	rBV4	490	392	0.02%	0.002%
58	7.568	1923	1937	1956	rBV	294741	519960	26.45%	3.098%
59	7.899	2027	2040	2059	rBV	881174	1637570	83.31%	9.758%
60	8.131	2109	2112	2115	rBV4	1244	1018	0.05%	0.006%
61	8.179	2116	2127	2153	rVV	203946	353828	18.00%	2.108%
62	8.349	2178	2180	2187	rBV6	852	893	0.05%	0.005%
63	8.555	2231	2244	2257	rBV	601491	1049160	53.37%	6.252%
64	8.632	2258	2268	2284	rBV	772849	1276811	64.96%	7.608%
65	9.005	2382	2384	2385	rBV3	338	134	0.01%	0.001%
66	9.015	2385	2387	2388	rVV3	329	101	0.01%	0.001%
67	9.108	2414	2416	2420	rBV4	773	543	0.03%	0.003%
68	9.160	2429	2432	2434	rBV3	1133	697	0.04%	0.004%
69	9.211	2446	2448	2450	rBV3	619	392	0.02%	0.002%
70	9.420	2498	2513	2540	rBV	724344	1287880	65.52%	7.674%
71	9.700	2589	2600	2608	rBV8	3801	7055	0.36%	0.042%
72	9.992	2685	2691	2693	rBV6	1333	1284	0.07%	0.008%
73	10.214	2756	2760	2764	rBV7	1310	1333	0.07%	0.008%
74	10.279	2777	2780	2783	rBV3	543	446	0.02%	0.003%
75	10.295	2783	2785	2787	rBV3	822	417	0.02%	0.002%
76	10.394	2814	2816	2818	rBV3	486	153	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047113.D
 Acq On : 11 Feb 2022 14:31
 Operator : SY/MD
 Sample : N1462-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M

Title : VOC Analysis

77	10.439	2826	2830	2831	rBV4	666	459	0.02%	0.003%
78	10.478	2838	2842	2843	rBV4	1163	731	0.04%	0.004%
79	10.594	2876	2878	2883	rVB7	1195	833	0.04%	0.005%
80	10.677	2895	2904	2912	rVB5	4387	7807	0.40%	0.047%
81	10.758	2915	2929	2950	rBV	651787	1060753	53.96%	6.321%
82	11.295	3093	3096	3099	rBV5	639	510	0.03%	0.003%
83	11.394	3124	3127	3130	rBV4	713	547	0.03%	0.003%
84	11.812	3243	3257	3273	rBV	825403	1317821	67.04%	7.853%
85	12.195	3363	3376	3391	rVB	927069	1508624	76.75%	8.990%
86	12.513	3472	3475	3476	rBV3	885	541	0.03%	0.003%
87	13.751	3856	3860	3863	rBV4	991	828	0.04%	0.005%




Sum of corrected areas: 16781845

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047113.D
Acq On : 11 Feb 2022 14:31
Operator : SY/MD
Sample : N1462-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

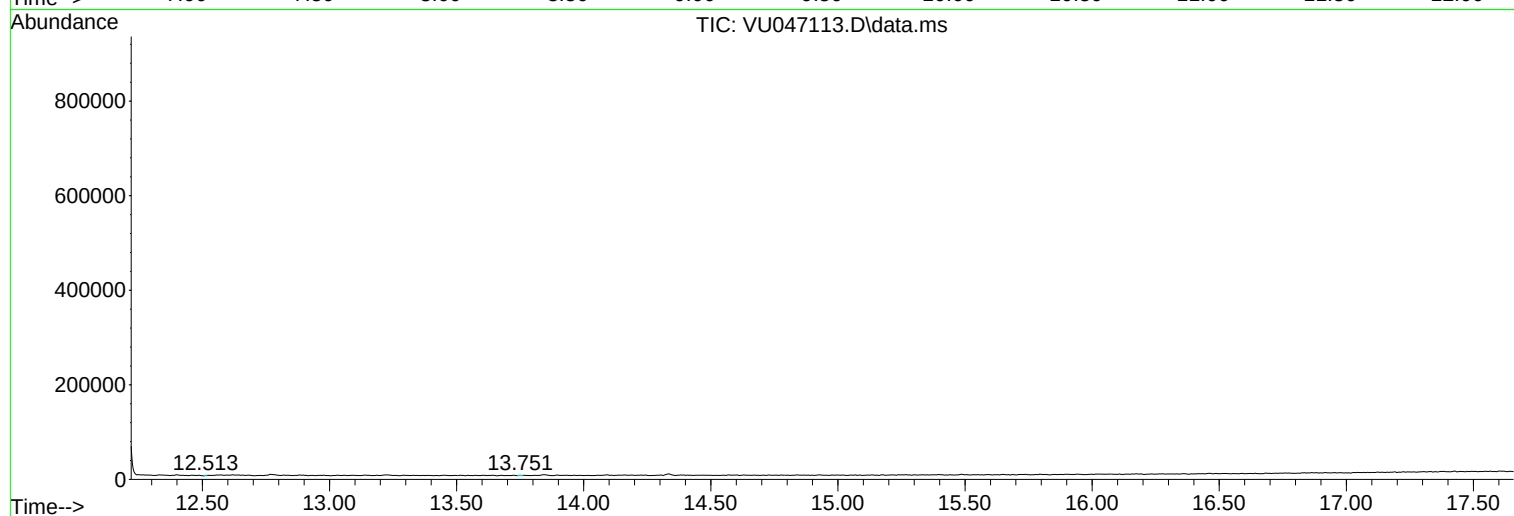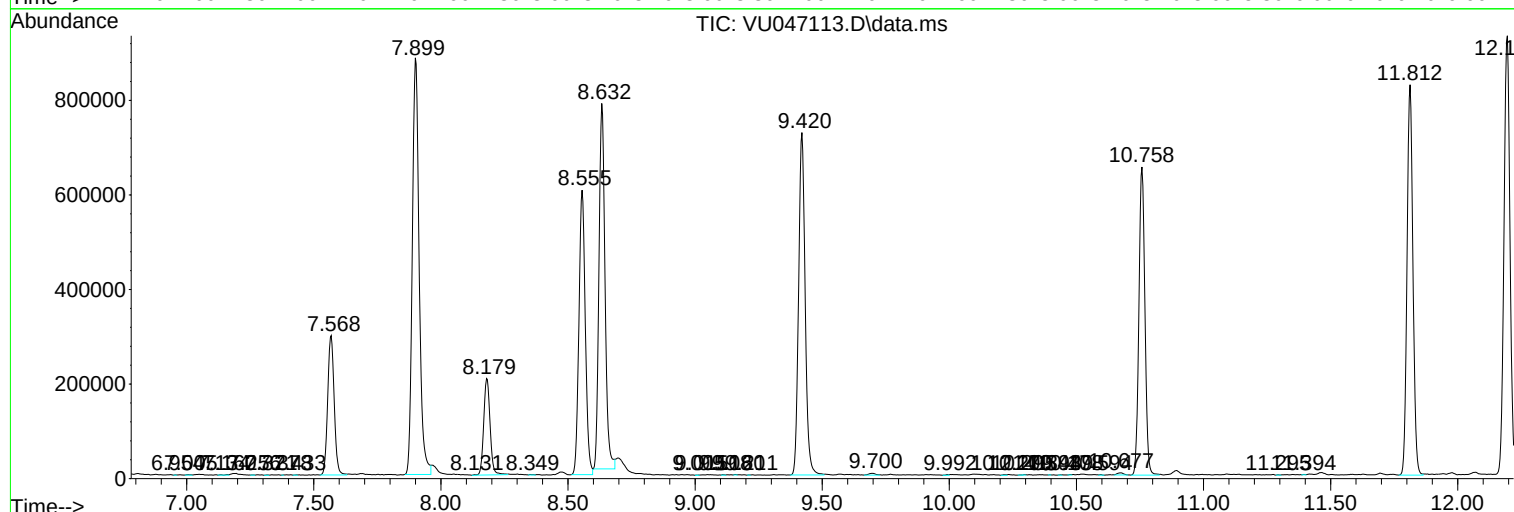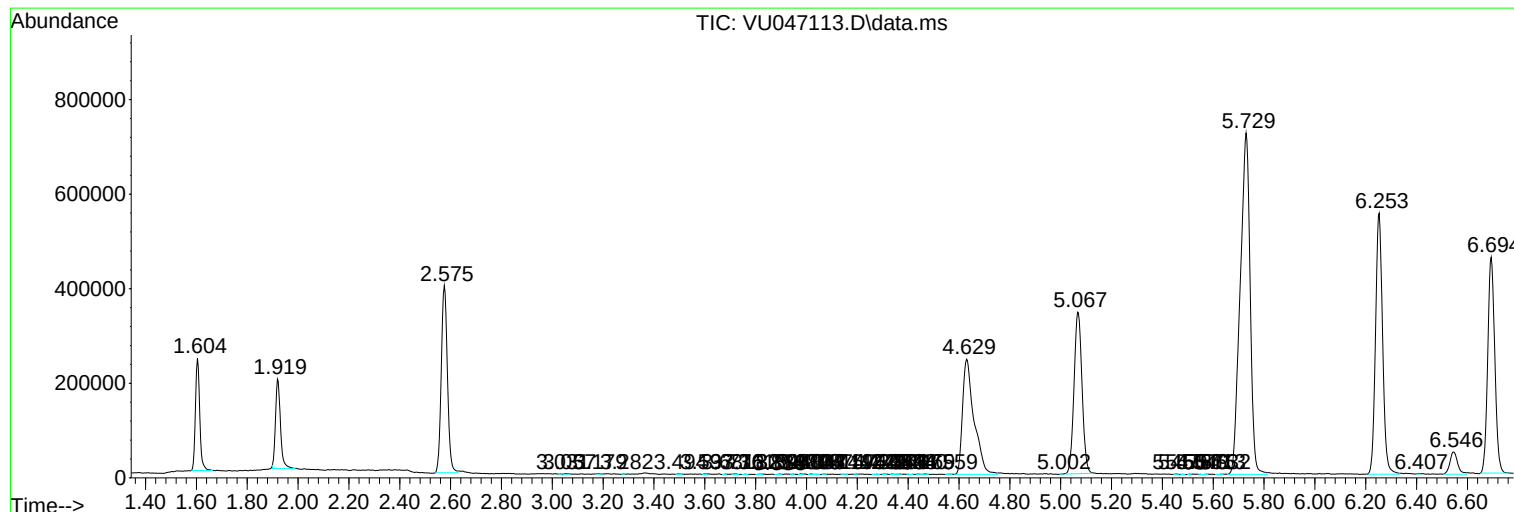

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047113.D
Acq On : 11 Feb 2022 14:31
Operator : SY/MD
Sample : N1462-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047113.D
Acq On : 11 Feb 2022 14:31
Operator : SY/MD
Sample : N1462-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------