

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047114.D
 Acq On : 11 Feb 2022 14:53
 Operator : SY/MD
 Sample : N1462-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M20DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.607	74	83	107	rBV2	556848	700891	37.61%	4.593%
2	1.919	173	180	195	rBV	175947	237359	12.74%	1.555%
3	2.575	372	384	402	rBV	372506	627091	33.65%	4.109%
4	2.761	440	442	446	rVB4	1682	1058	0.06%	0.007%
5	2.797	451	453	458	rVV6	1451	1097	0.06%	0.007%
6	2.829	461	463	467	rVB5	1034	647	0.03%	0.004%
7	2.883	477	480	484	rBV7	714	606	0.03%	0.004%
8	3.057	530	534	537	rBV5	1126	823	0.04%	0.005%
9	3.108	545	550	553	rBV8	1083	886	0.05%	0.006%
10	3.189	568	575	578	rBV6	2900	4015	0.22%	0.026%
11	3.298	607	609	615	rVB7	825	726	0.04%	0.005%
12	3.340	615	622	623	rBV5	770	816	0.04%	0.005%
13	3.359	624	628	634	rVB8	1076	1267	0.07%	0.008%
14	3.694	729	732	738	rBV6	660	663	0.04%	0.004%
15	3.838	775	777	781	rVB4	924	693	0.04%	0.005%
16	4.012	824	831	837	rVB7	1509	1789	0.10%	0.012%
17	4.182	881	884	889	rVB7	1102	930	0.05%	0.006%
18	4.215	889	894	898	rBV6	1124	955	0.05%	0.006%
19	4.327	927	929	936	rVB8	1206	998	0.05%	0.007%
20	4.498	980	982	986	rVB3	1210	672	0.04%	0.004%
21	4.633	1009	1024	1029	rBV	238332	511052	27.42%	3.349%
22	4.915	1108	1112	1119	rBV7	1128	1356	0.07%	0.009%
23	5.067	1144	1159	1178	rBV	326340	712542	38.24%	4.669%
24	5.208	1201	1203	1207	rBV5	1125	643	0.03%	0.004%
25	5.292	1223	1229	1230	rBV4	983	988	0.05%	0.006%
26	5.337	1238	1243	1245	rBV5	910	649	0.03%	0.004%
27	5.398	1258	1262	1264	rBV4	877	702	0.04%	0.005%
28	5.607	1324	1327	1330	rBV3	1149	935	0.05%	0.006%
29	5.729	1342	1365	1393	rBV2	687326	1863552	100.00%	12.212%
30	6.031	1454	1459	1462	rBV5	978	1029	0.06%	0.007%
31	6.108	1478	1483	1485	rBV6	1137	921	0.05%	0.006%
32	6.253	1513	1528	1560	rVV	516264	1021792	54.83%	6.696%
33	6.465	1590	1594	1598	rVB7	878	676	0.04%	0.004%
34	6.533	1607	1615	1617	rBV7	3445	4123	0.22%	0.027%
35	6.694	1651	1665	1689	rBV	434027	839522	45.05%	5.501%
36	6.899	1723	1729	1731	rBV5	1020	910	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047114.D
 Acq On : 11 Feb 2022 14:53
 Operator : SY/MD
 Sample : N1462-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M20DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	7.005	1757	1762	1763	rBV4	641	614	0.03%	0.004%
38	7.031	1766	1770	1771	rVV3	1141	813	0.04%	0.005%
39	7.054	1771	1777	1783	rVV8	2206	3260	0.17%	0.021%
40	7.099	1789	1791	1795	rVV4	1119	723	0.04%	0.005%
41	7.144	1800	1805	1809	rBV7	775	1040	0.06%	0.007%
42	7.189	1809	1819	1834	rVV7	3328	7158	0.38%	0.047%
43	7.243	1834	1836	1841	rVB5	864	657	0.04%	0.004%
44	7.346	1862	1868	1870	rBV6	1079	1015	0.05%	0.007%
45	7.385	1876	1880	1883	rBV4	899	757	0.04%	0.005%
46	7.414	1886	1889	1895	rBV7	912	998	0.05%	0.007%
47	7.568	1924	1937	1955	rBV	281162	490950	26.34%	3.217%
48	7.784	2000	2004	2005	rBV4	864	627	0.03%	0.004%
49	7.899	2023	2040	2059	rBV	829670	1565319	84.00%	10.258%
50	8.179	2114	2127	2149	rBV	195867	332382	17.84%	2.178%
51	8.391	2189	2193	2198	rVV7	641	589	0.03%	0.004%
52	8.472	2208	2218	2228	rVB2	3828	7314	0.39%	0.048%
53	8.552	2235	2243	2253	rBV10	3507	5984	0.32%	0.039%
54	8.632	2256	2268	2283	rBV	745505	1268886	68.09%	8.315%
55	8.970	2371	2373	2376	rVB4	1323	611	0.03%	0.004%
56	9.086	2405	2409	2413	rBV6	951	1070	0.06%	0.007%
57	9.221	2444	2451	2455	rBV9	1216	1476	0.08%	0.010%
58	9.250	2456	2460	2463	rBV6	969	673	0.04%	0.004%
59	9.311	2475	2479	2482	rVB4	832	586	0.03%	0.004%
60	9.420	2499	2513	2537	rBV	682727	1232655	66.15%	8.078%
61	9.568	2555	2559	2560	rBV3	1143	832	0.04%	0.005%
62	9.693	2591	2598	2607	rVV4	4560	7620	0.41%	0.050%
63	10.163	2741	2744	2751	rVB8	1134	1056	0.06%	0.007%
64	10.198	2751	2755	2757	rBV2	1053	808	0.04%	0.005%
65	10.484	2838	2844	2847	rBV7	1480	1833	0.10%	0.012%
66	10.645	2889	2894	2895	rBV5	870	739	0.04%	0.005%
67	10.674	2895	2903	2914	rVB4	4430	8115	0.44%	0.053%
68	10.758	2915	2929	2947	rBV	624180	1012246	54.32%	6.633%
69	10.893	2966	2971	2987	rVB5	5440	10307	0.55%	0.068%
70	10.960	2989	2992	2996	rBV4	1043	608	0.03%	0.004%
71	11.082	3026	3030	3031	rBV4	1102	781	0.04%	0.005%
72	11.288	3088	3094	3096	rBV6	734	584	0.03%	0.004%
73	11.398	3124	3128	3129	rBV3	728	571	0.03%	0.004%
74	11.410	3129	3132	3137	rVB4	1963	1573	0.08%	0.010%
75	11.462	3143	3148	3161	rVB6	5422	8964	0.48%	0.059%
76	11.574	3178	3183	3184	rBV5	1205	992	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047114.D
 Acq On : 11 Feb 2022 14:53
 Operator : SY/MD
 Sample : N1462-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M20DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	11.632	3196	3201	3203	rBV5	1110	971	0.05%	0.006%
78	11.693	3214	3220	3226	rVV7	2093	2950	0.16%	0.019%
79	11.812	3244	3257	3278	rBV	789486	1253345	67.26%	8.213%
80	12.063	3331	3335	3338	rBV4	1236	1183	0.06%	0.008%
81	12.192	3359	3375	3393	rBV	897039	1449156	77.76%	9.496%
82	12.333	3414	3419	3426	rVB10	1663	2235	0.12%	0.015%
83	12.877	3584	3588	3591	rBV5	1108	962	0.05%	0.006%
84	13.137	3664	3669	3670	rBV5	1153	843	0.05%	0.006%
85	13.205	3686	3690	3691	rBV4	1038	656	0.04%	0.004%
86	13.221	3691	3695	3702	rVB6	1895	1920	0.10%	0.013%
87	13.330	3725	3729	3732	rBV6	1253	925	0.05%	0.006%
88	13.349	3732	3735	3740	rVB6	878	727	0.04%	0.005%
89	13.516	3784	3787	3790	rBV4	753	616	0.03%	0.004%
90	13.677	3831	3837	3842	rVB9	1195	1298	0.07%	0.009%
91	13.732	3847	3854	3856	rBV7	1124	1090	0.06%	0.007%
92	13.838	3880	3887	3891	rBV8	1486	2240	0.12%	0.015%
93	14.079	3959	3962	3967	rBV6	943	852	0.05%	0.006%
94	14.333	4036	4041	4044	rBV6	1882	1760	0.09%	0.012%
95	14.574	4112	4116	4120	rBV6	1359	1266	0.07%	0.008%
96	14.764	4173	4175	4180	rVB3	1026	815	0.04%	0.005%
97	14.803	4180	4187	4191	rVB7	1710	2270	0.12%	0.015%
98	14.828	4191	4195	4197	rBV3	1415	1239	0.07%	0.008%
99	14.938	4226	4229	4232	rVB5	1645	1029	0.06%	0.007%
100	15.143	4291	4293	4296	rVB4	957	598	0.03%	0.004%




Sum of corrected areas: 15260106

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047114.D
Acq On : 11 Feb 2022 14:53
Operator : SY/MD
Sample : N1462-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M20DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

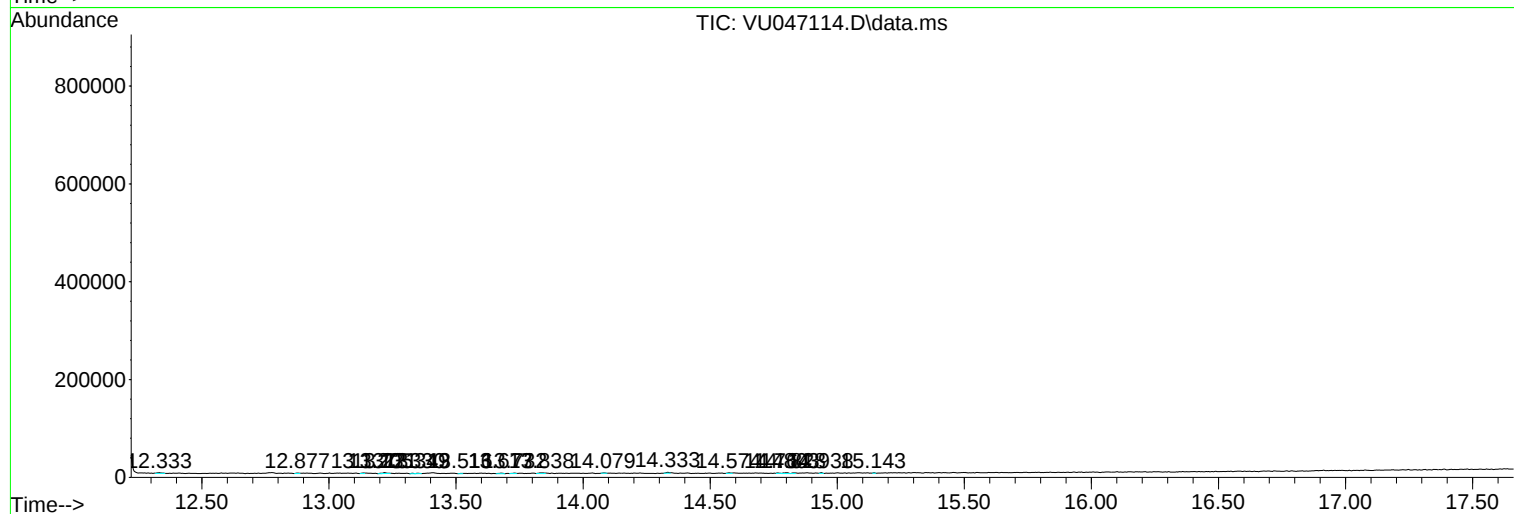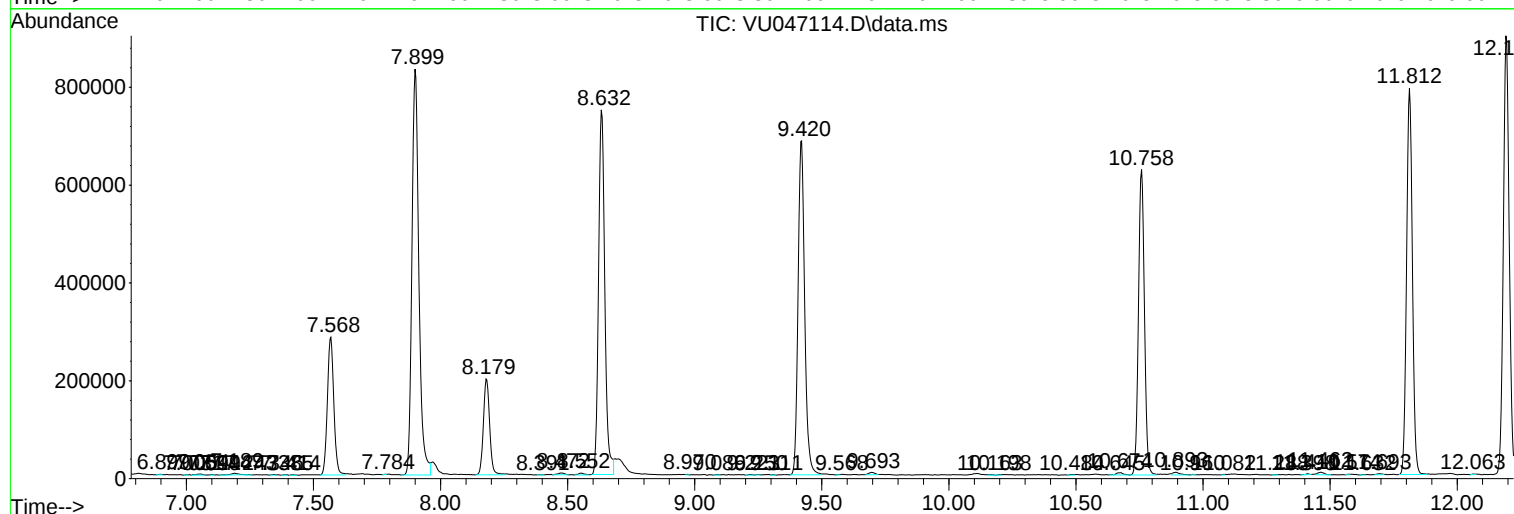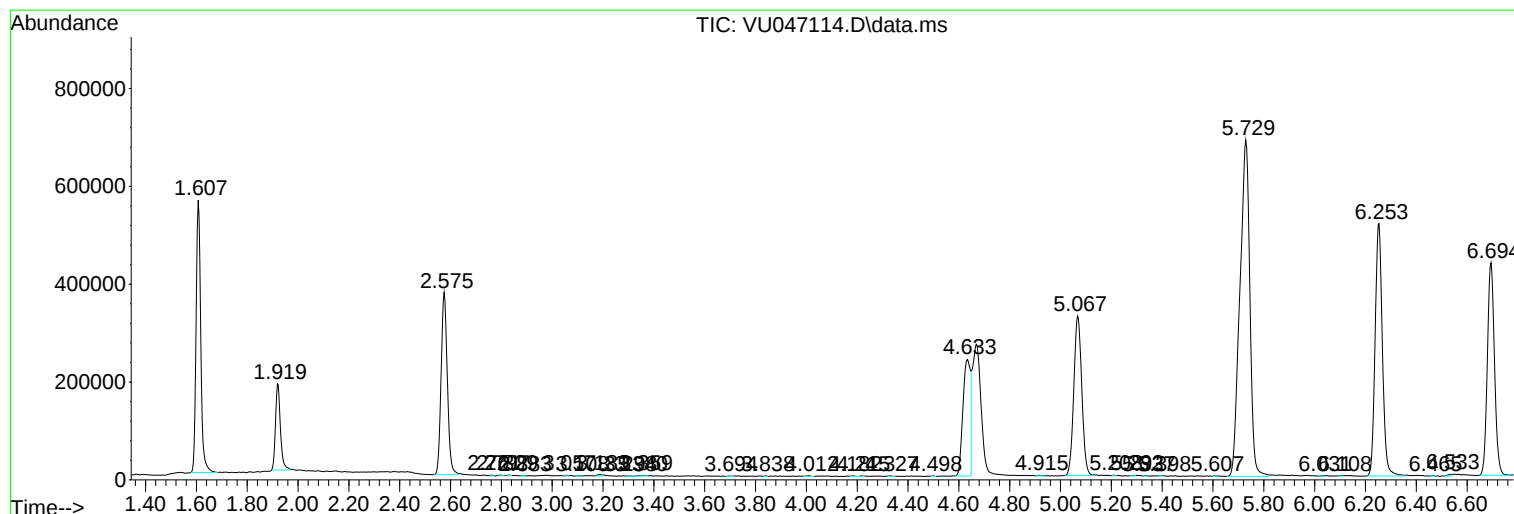

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047114.D
Acq On : 11 Feb 2022 14:53
Operator : SY/MD
Sample : N1462-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M20DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047114.D
Acq On : 11 Feb 2022 14:53
Operator : SY/MD
Sample : N1462-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M20DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------