

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047116.D
 Acq On : 11 Feb 2022 15:38
 Operator : SY/MD
 Sample : N1462-04DL 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M31DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M

Title : VOC Analysis

Signal : TIC: VU047116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.607	74	83	100	rBV2	308031	390040	20.91%	2.380%
2	1.919	172	180	202	rBV	176702	248751	13.33%	1.518%
3	2.575	372	384	411	rVB	371667	627863	33.66%	3.831%
4	2.768	442	444	448	rVB5	1528	690	0.04%	0.004%
5	3.028	522	525	528	rBV4	1067	969	0.05%	0.006%
6	3.048	528	531	533	rBV4	909	733	0.04%	0.004%
7	3.115	546	552	554	rBV6	804	975	0.05%	0.006%
8	3.176	566	571	572	rBV4	1542	1444	0.08%	0.009%
9	3.369	618	631	637	rVV9	3763	7249	0.39%	0.044%
10	3.440	647	653	656	rBV6	911	872	0.05%	0.005%
11	3.533	677	682	688	rVB9	632	838	0.04%	0.005%
12	3.565	688	692	695	rBV4	887	667	0.04%	0.004%
13	3.681	722	728	731	rBV8	824	774	0.04%	0.005%
14	3.707	732	736	739	rVB6	1081	681	0.04%	0.004%
15	3.986	817	823	826	rBV4	1021	1049	0.06%	0.006%
16	4.009	826	830	833	rVV5	695	606	0.03%	0.004%
17	4.112	856	862	865	rBV6	878	973	0.05%	0.006%
18	4.160	873	877	884	rVB8	756	937	0.05%	0.006%
19	4.205	884	891	897	rVB9	1177	1652	0.09%	0.010%
20	4.244	897	903	906	rBV7	949	974	0.05%	0.006%
21	4.382	943	946	950	rVV4	963	758	0.04%	0.005%
22	4.456	965	969	973	rVB5	784	654	0.04%	0.004%
23	4.485	973	978	981	rBV3	874	719	0.04%	0.004%
24	4.504	981	984	989	rVV8	601	607	0.03%	0.004%
25	4.671	1009	1036	1057	rBV2	585905	1845604	98.93%	11.262%
26	5.067	1142	1159	1177	rBV	328379	710537	38.09%	4.336%
27	5.279	1222	1225	1231	rBV7	872	963	0.05%	0.006%
28	5.305	1231	1233	1237	rBV4	801	659	0.04%	0.004%
29	5.382	1249	1257	1259	rBV7	1242	1285	0.07%	0.008%
30	5.469	1282	1284	1292	rVB7	1414	1367	0.07%	0.008%
31	5.510	1292	1297	1301	rBV7	1152	1477	0.08%	0.009%
32	5.572	1310	1316	1320	rBV6	633	882	0.05%	0.005%
33	5.729	1341	1365	1389	rBV2	679680	1865501	100.00%	11.384%
34	6.038	1456	1461	1462	rBV4	1137	913	0.05%	0.006%
35	6.250	1513	1527	1553	rVV	519437	1018530	54.60%	6.215%
36	6.546	1606	1619	1633	rBV	54735	110644	5.93%	0.675%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047116.D
 Acq On : 11 Feb 2022 15:38
 Operator : SY/MD
 Sample : N1462-04DL 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M31DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	6.694	1650	1665	1684	rBV	433075	851680	45.65%	5.197%
38	7.047	1769	1775	1781	rBV8	953	1364	0.07%	0.008%
39	7.144	1803	1805	1810	rBV4	930	767	0.04%	0.005%
40	7.186	1810	1818	1824	rBV8	3577	5727	0.31%	0.035%
41	7.462	1900	1904	1910	rBV7	931	881	0.05%	0.005%
42	7.568	1923	1937	1951	rBV	276537	492787	26.42%	3.007%
43	7.694	1970	1976	1984	rVB	1869	2793	0.15%	0.017%
44	7.899	2026	2040	2059	rBV	842607	1553012	83.25%	9.477%
45	8.083	2094	2097	2103	rVB6	1131	1193	0.06%	0.007%
46	8.137	2110	2114	2116	rBV4	908	746	0.04%	0.005%
47	8.179	2116	2127	2154	rVV	191635	332462	17.82%	2.029%
48	8.475	2208	2219	2229	rBV2	5415	9931	0.53%	0.061%
49	8.555	2233	2244	2255	rBV2	33587	56603	3.03%	0.345%
50	8.633	2256	2268	2283	rBV	735934	1256417	67.35%	7.667%
51	9.063	2397	2402	2405	rVB5	847	731	0.04%	0.004%
52	9.166	2431	2434	2439	rVB4	1271	961	0.05%	0.006%
53	9.260	2460	2463	2466	rBV3	907	731	0.04%	0.004%
54	9.298	2471	2475	2478	rVB4	934	686	0.04%	0.004%
55	9.420	2499	2513	2539	rBV	695121	1221734	65.49%	7.455%
56	9.552	2551	2554	2558	rVB5	1468	939	0.05%	0.006%
57	9.575	2558	2561	2564	rBV5	890	602	0.03%	0.004%
58	9.597	2564	2568	2574	rVB7	1095	1129	0.06%	0.007%
59	9.639	2574	2581	2584	rBV7	1092	1425	0.08%	0.009%
60	9.697	2592	2599	2606	rVB6	2464	3722	0.20%	0.023%
61	9.729	2606	2609	2614	rVB5	1247	1210	0.06%	0.007%
62	9.771	2620	2622	2627	rBV4	810	676	0.04%	0.004%
63	9.841	2638	2644	2647	rBV6	1210	1351	0.07%	0.008%
64	10.099	2717	2724	2727	rBV8	1850	2300	0.12%	0.014%
65	10.198	2750	2755	2757	rBV5	810	878	0.05%	0.005%
66	10.301	2783	2787	2792	rVB6	867	700	0.04%	0.004%
67	10.366	2805	2807	2813	rBV8	871	776	0.04%	0.005%
68	10.488	2842	2845	2849	rVB6	1618	1128	0.06%	0.007%
69	10.671	2894	2902	2909	rVB4	4562	6659	0.36%	0.041%
70	10.758	2916	2929	2945	rBV	619930	1008930	54.08%	6.157%
71	11.070	3023	3026	3030	rBV4	805	615	0.03%	0.004%
72	11.153	3050	3052	3060	rVB6	1756	1703	0.09%	0.010%
73	11.198	3062	3066	3068	rBV3	1019	889	0.05%	0.005%
74	11.462	3140	3148	3158	rVB8	4794	8318	0.45%	0.051%
75	11.645	3203	3205	3211	rVV7	1215	1076	0.06%	0.007%
76	11.697	3211	3221	3228	rVV10	3098	4602	0.25%	0.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047116.D
 Acq On : 11 Feb 2022 15:38
 Operator : SY/MD
 Sample : N1462-04DL 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M31DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	11.742	3233	3235	3244	rVB8	1282	1379	0.07%	0.008%
78	11.812	3244	3257	3273	rBV	781073	1243124	66.64%	7.586%
79	12.025	3320	3323	3328	rVB6	1068	895	0.05%	0.005%
80	12.086	3337	3342	3344	rBV6	1157	791	0.04%	0.005%
81	12.195	3362	3376	3392	rVV	871623	1432370	76.78%	8.741%
82	12.327	3412	3417	3418	rBV4	1322	1010	0.05%	0.006%
83	12.456	3452	3457	3460	rBV8	662	832	0.04%	0.005%
84	12.513	3472	3475	3477	rBV3	1013	640	0.03%	0.004%
85	12.819	3566	3570	3571	rBV2	892	592	0.03%	0.004%
86	13.115	3658	3662	3667	rVB6	1204	1007	0.05%	0.006%
87	13.137	3667	3669	3671	rBV3	1120	702	0.04%	0.004%
88	13.224	3691	3696	3699	rVV6	980	946	0.05%	0.006%
89	13.401	3748	3751	3754	rBV3	898	652	0.03%	0.004%
90	13.822	3879	3882	3885	rBV4	931	913	0.05%	0.006%
91	13.838	3885	3887	3894	rVB7	1628	1696	0.09%	0.010%
92	13.996	3934	3936	3942	rVB8	867	723	0.04%	0.004%
93	14.041	3948	3950	3955	rVB5	946	676	0.04%	0.004%
94	14.156	3982	3986	3992	rVB7	945	922	0.05%	0.006%
95	14.189	3992	3996	4000	rBV4	1038	1121	0.06%	0.007%
96	14.298	4027	4030	4034	rBV3	735	626	0.03%	0.004%
97	14.333	4038	4041	4048	rVB7	1663	2046	0.11%	0.012%
98	14.365	4048	4051	4058	rBV10	953	827	0.04%	0.005%
99	14.423	4067	4069	4073	rBV4	885	641	0.03%	0.004%
100	14.574	4111	4116	4119	rBV5	1776	1546	0.08%	0.009%




Sum of corrected areas: 16387348

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047116.D
Acq On : 11 Feb 2022 15:38
Operator : SY/MD
Sample : N1462-04DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M31DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

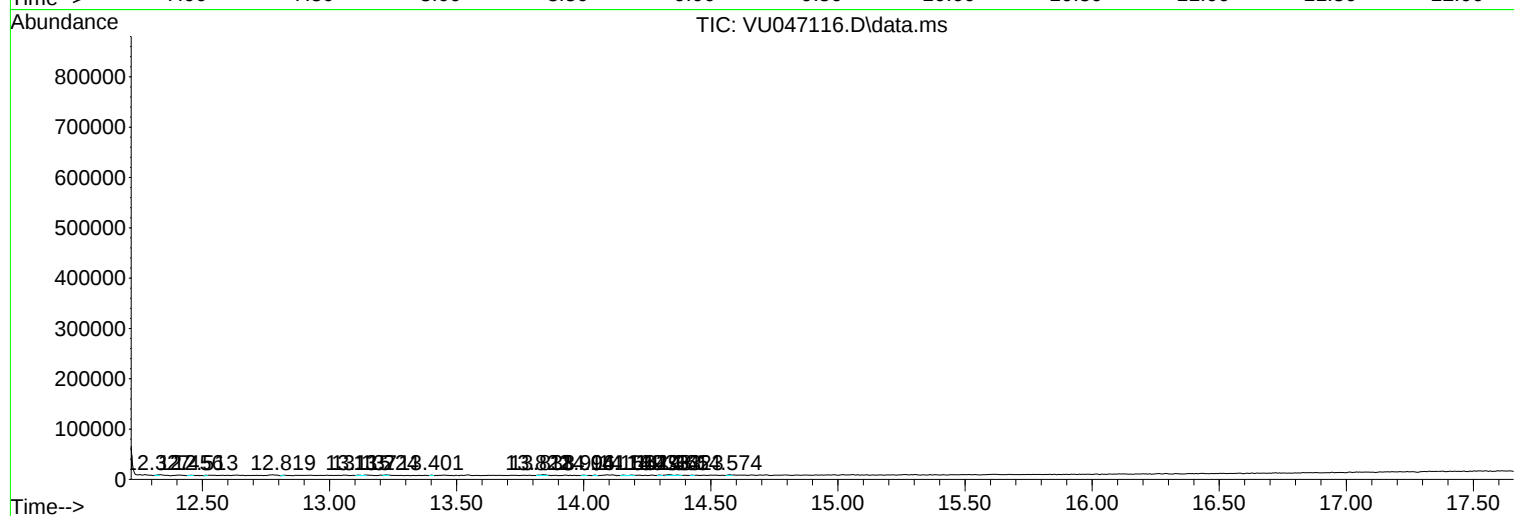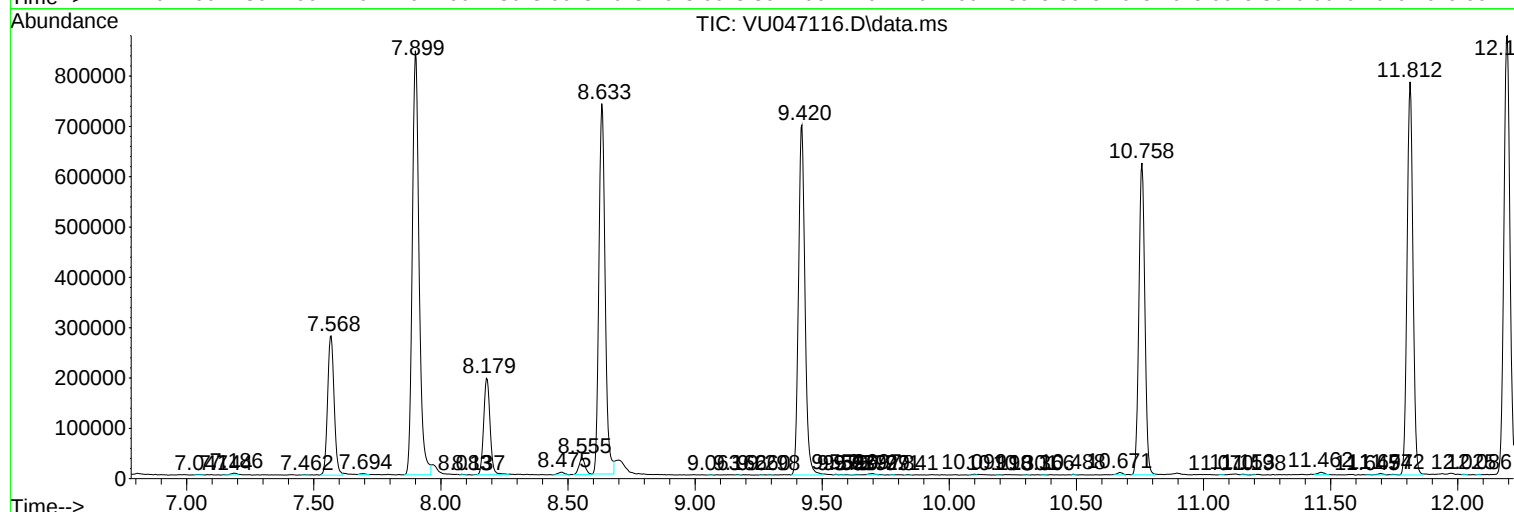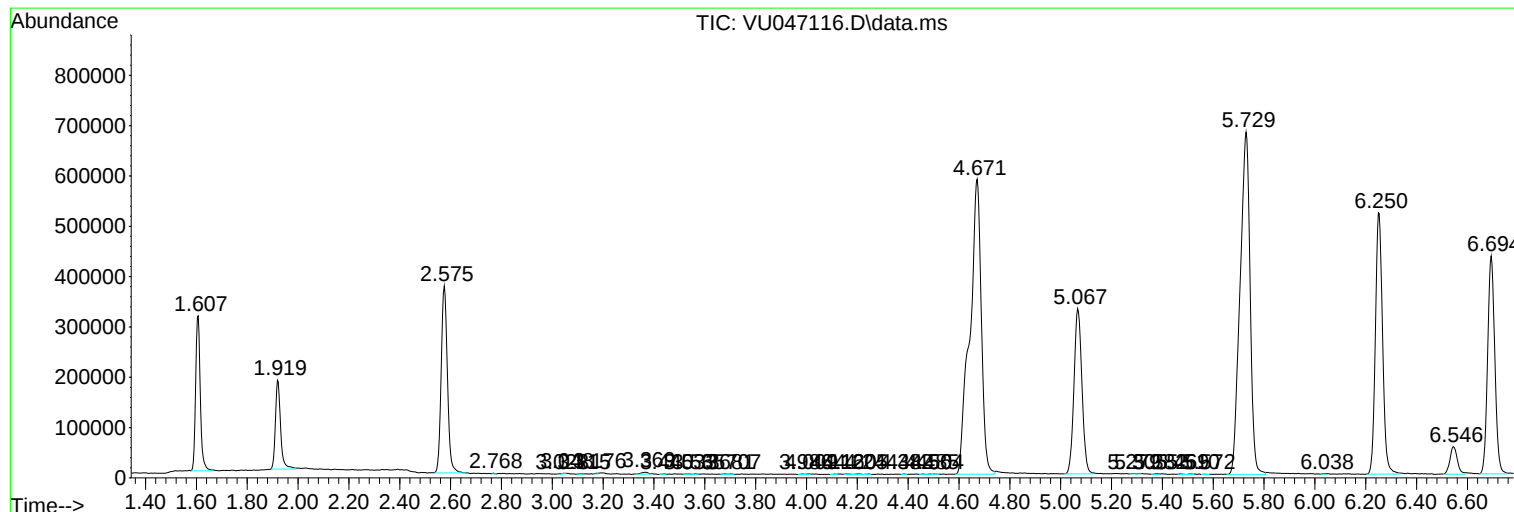

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047116.D
Acq On : 11 Feb 2022 15:38
Operator : SY/MD
Sample : N1462-04DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M31DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047116.D
Acq On : 11 Feb 2022 15:38
Operator : SY/MD
Sample : N1462-04DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M31DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------