

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047117.D
 Acq On : 11 Feb 2022 16:01
 Operator : SY/MD
 Sample : N1462-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.607	75	83	106	rBV2	513697	647972	27.42%	3.774%
2	1.919	174	180	201	rVB	172025	232557	9.84%	1.354%
3	2.575	372	384	401	rBV	368623	620967	26.27%	3.617%
4	3.363	621	629	654	rVB4	40353	85540	3.62%	0.498%
5	3.456	654	658	659	rBV3	707	585	0.02%	0.003%
6	3.546	683	686	691	rBV3	542	517	0.02%	0.003%
7	3.803	762	766	768	rBV5	776	571	0.02%	0.003%
8	3.928	802	805	808	rBV4	576	430	0.02%	0.003%
9	3.967	814	817	820	rVB5	1268	797	0.03%	0.005%
10	4.002	820	828	834	rVB7	1581	2294	0.10%	0.013%
11	4.031	834	837	840	rBV4	754	632	0.03%	0.004%
12	4.051	840	843	845	rBV4	479	273	0.01%	0.002%
13	4.147	869	873	874	rBV3	590	294	0.01%	0.002%
14	4.199	887	889	890	rBV2	458	232	0.01%	0.001%
15	4.237	899	901	903	rBV3	578	268	0.01%	0.002%
16	4.253	903	906	907	rBV3	745	379	0.02%	0.002%
17	4.285	913	916	921	rBV6	613	448	0.02%	0.003%
18	4.327	926	929	932	rVB3	949	562	0.02%	0.003%
19	4.346	932	935	938	rBV4	577	419	0.02%	0.002%
20	4.411	950	955	958	rBV5	584	638	0.03%	0.004%
21	4.465	966	972	976	rBV8	683	840	0.04%	0.005%
22	4.533	991	993	997	rVB4	1011	574	0.02%	0.003%
23	4.568	999	1004	1007	rBV7	1282	1317	0.06%	0.008%
24	4.671	1009	1036	1073	rVV2	811755	2363400	100.00%	13.765%
25	5.067	1144	1159	1181	rBV	324043	711502	30.11%	4.144%
26	5.507	1293	1296	1299	rBV4	750	626	0.03%	0.004%
27	5.581	1316	1319	1323	rBV4	824	596	0.03%	0.003%
28	5.729	1343	1365	1396	rBV2	677849	1864404	78.89%	10.859%
29	6.118	1482	1486	1488	rBV4	1359	939	0.04%	0.005%
30	6.253	1513	1528	1556	rBV	541242	1065342	45.08%	6.205%
31	6.491	1600	1602	1604	rBV2	467	243	0.01%	0.001%
32	6.694	1652	1665	1689	rVB	433428	834626	35.31%	4.861%
33	6.983	1754	1755	1761	rBV6	595	485	0.02%	0.003%
34	7.038	1769	1772	1773	rBV4	810	481	0.02%	0.003%
35	7.141	1800	1804	1806	rBV5	747	594	0.03%	0.003%
36	7.337	1863	1865	1869	rBV4	560	428	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047117.D
 Acq On : 11 Feb 2022 16:01
 Operator : SY/MD
 Sample : N1462-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4M26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	7.385	1877	1880	1881	rBV2	485	300	0.01%	0.002%
38	7.424	1889	1892	1893	rBV3	682	395	0.02%	0.002%
39	7.568	1924	1937	1954	rBV	274380	485261	20.53%	2.826%
40	7.899	2027	2040	2059	rBV	817265	1546294	65.43%	9.006%
41	8.179	2115	2127	2146	rBV	192804	330323	13.98%	1.924%
42	8.632	2256	2268	2284	rBV	748173	1285275	54.38%	7.486%
43	8.858	2336	2338	2344	rVB7	994	925	0.04%	0.005%
44	8.890	2344	2348	2350	rBV5	730	580	0.02%	0.003%
45	8.983	2374	2377	2380	rBV4	1007	606	0.03%	0.004%
46	8.999	2380	2382	2386	rVV3	664	535	0.02%	0.003%
47	9.067	2399	2403	2404	rBV3	927	528	0.02%	0.003%
48	9.108	2413	2416	2417	rBV2	551	293	0.01%	0.002%
49	9.208	2441	2447	2450	rBV2	772	826	0.03%	0.005%
50	9.269	2463	2466	2469	rBV3	572	371	0.02%	0.002%
51	9.372	2492	2498	2499	rBV6	1334	1214	0.05%	0.007%
52	9.420	2500	2513	2538	rVV	716779	1281557	54.23%	7.464%
53	9.803	2630	2632	2636	rBV3	776	482	0.02%	0.003%
54	10.218	2756	2761	2766	rBV6	1145	1493	0.06%	0.009%
55	10.295	2781	2785	2787	rBV3	761	630	0.03%	0.004%
56	10.536	2857	2860	2862	rBV5	703	425	0.02%	0.002%
57	10.645	2889	2894	2896	rBV5	1289	1255	0.05%	0.007%
58	10.758	2917	2929	2947	rBV	622917	1010200	42.74%	5.884%
59	10.973	2993	2996	2998	rBV3	803	538	0.02%	0.003%
60	11.054	3019	3021	3026	rBV3	733	571	0.02%	0.003%
61	11.176	3057	3059	3061	rVB3	808	281	0.01%	0.002%
62	11.195	3062	3065	3068	rBV5	1217	917	0.04%	0.005%
63	11.465	3140	3149	3163	rVB6	4821	9647	0.41%	0.056%
64	11.629	3197	3200	3202	rBV4	542	364	0.02%	0.002%
65	11.690	3214	3219	3220	rBV4	2623	2037	0.09%	0.012%
66	11.745	3231	3236	3243	rBV8	1655	2387	0.10%	0.014%
67	11.812	3244	3257	3274	rVV	831305	1307528	55.32%	7.615%
68	12.070	3325	3337	3346	rBV5	4241	9203	0.39%	0.054%
69	12.195	3363	3376	3396	rVB	873764	1440020	60.93%	8.387%
70	12.478	3460	3464	3466	rBV4	1371	908	0.04%	0.005%
71	12.877	3584	3588	3589	rBV3	1054	673	0.03%	0.004%
72	12.989	3621	3623	3626	rBV4	880	612	0.03%	0.004%
73	13.250	3702	3704	3708	rBV3	680	349	0.01%	0.002%
74	13.613	3814	3817	3819	rBV4	787	437	0.02%	0.003%
75	13.777	3865	3868	3871	rBV6	1089	892	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047117.D
Acq On : 11 Feb 2022 16:01
Operator : SY/MD
Sample : N1462-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M26

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Title : VOC Analysis




Sum of corrected areas: 17169904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047117.D
Acq On : 11 Feb 2022 16:01
Operator : SY/MD
Sample : N1462-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

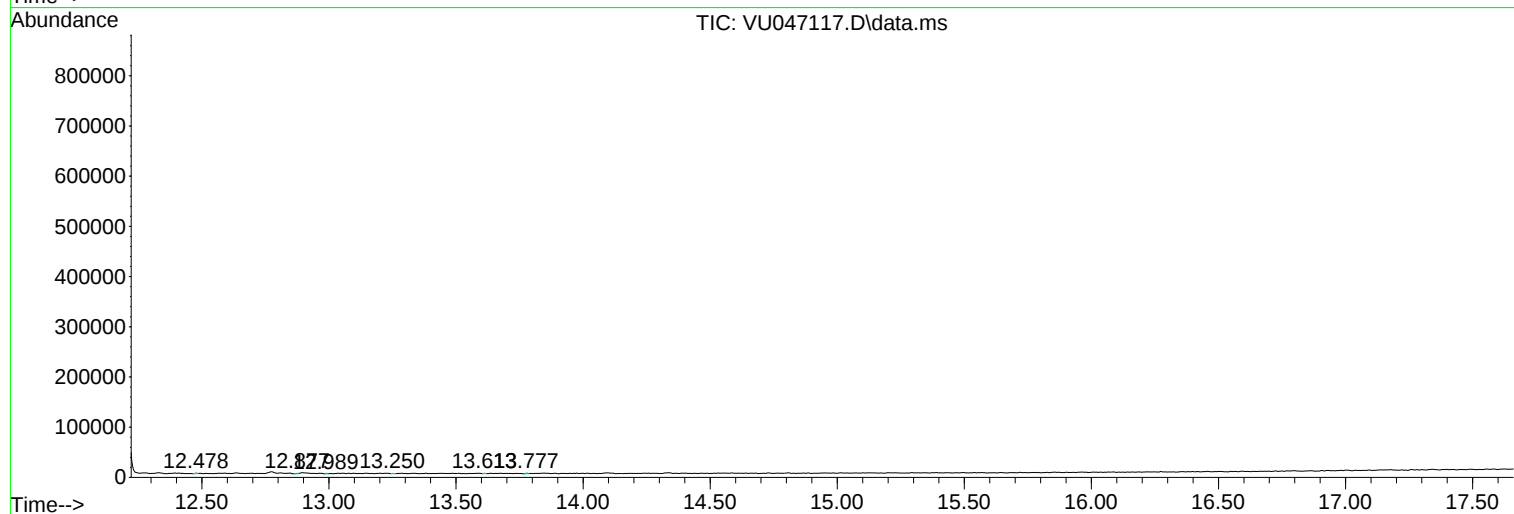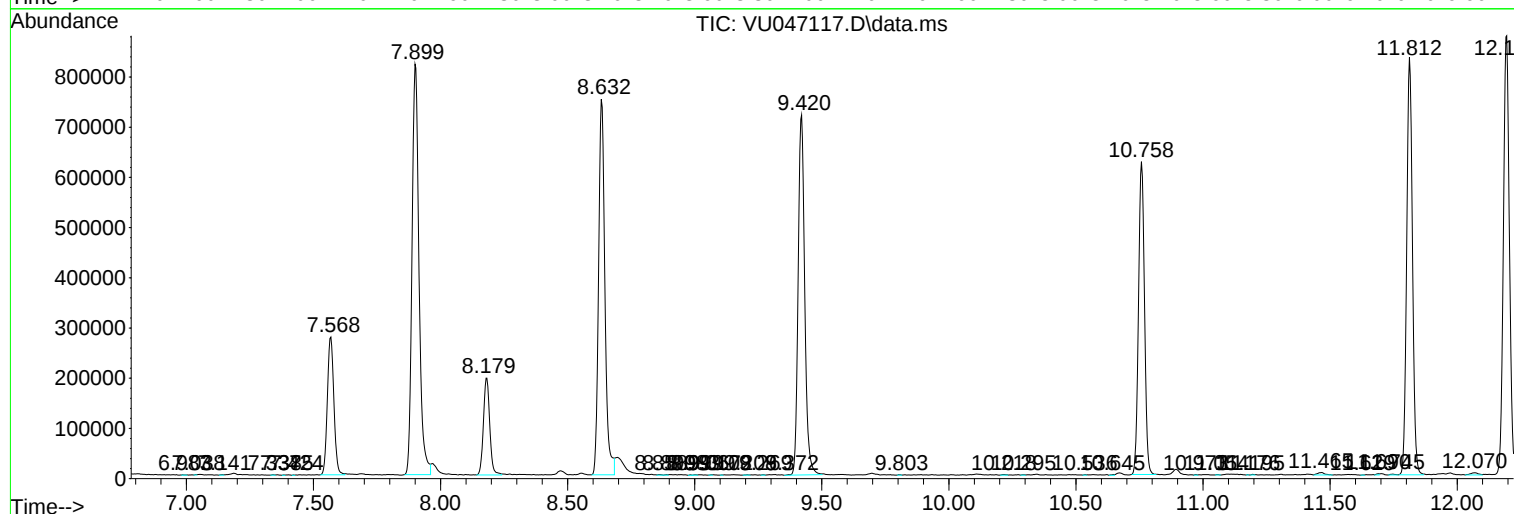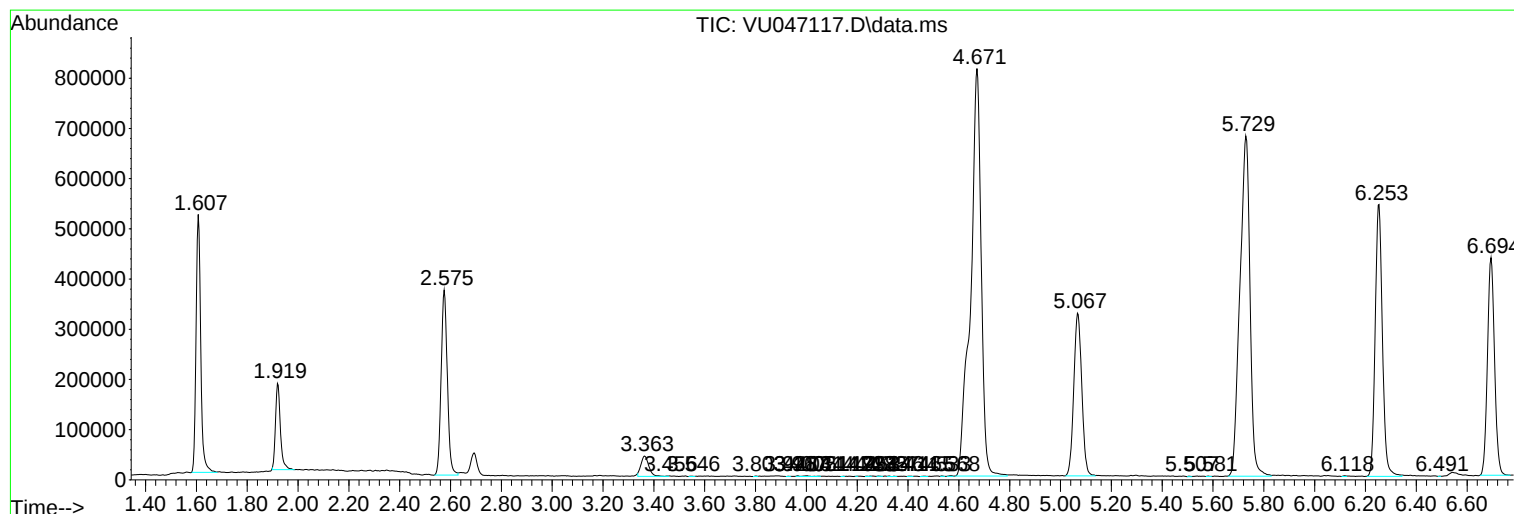

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047117.D
Acq On : 11 Feb 2022 16:01
Operator : SY/MD
Sample : N1462-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047117.D
Acq On : 11 Feb 2022 16:01
Operator : SY/MD
Sample : N1462-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4M26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------