

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047119.D
 Acq On : 11 Feb 2022 16:46
 Operator : SY/MD
 Sample : N1474-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	99	rBV	236523	277226	14.64%	1.857%
2	1.919	172	180	209	rVB	188662	263386	13.91%	1.764%
3	2.575	370	384	400	rBV	386921	650281	34.35%	4.355%
4	2.790	445	451	457	rBV8	955	1497	0.08%	0.010%
5	3.051	526	532	544	rVB8	1870	4011	0.21%	0.027%
6	3.105	544	549	551	rBV5	1024	781	0.04%	0.005%
7	3.166	565	568	570	rBV3	790	522	0.03%	0.003%
8	3.372	629	632	636	rVB5	865	550	0.03%	0.004%
9	3.398	636	640	643	rBV5	682	615	0.03%	0.004%
10	3.665	719	723	727	rVB5	913	920	0.05%	0.006%
11	3.707	731	736	738	rBV5	1085	1182	0.06%	0.008%
12	3.932	804	806	811	rBV5	781	745	0.04%	0.005%
13	4.131	863	868	871	rVV5	990	998	0.05%	0.007%
14	4.157	871	876	881	rVB6	675	599	0.03%	0.004%
15	4.192	883	887	889	rBV3	799	552	0.03%	0.004%
16	4.353	934	937	942	rBV6	771	756	0.04%	0.005%
17	4.629	1008	1023	1054	rBV	224133	584051	30.85%	3.911%
18	5.002	1136	1139	1141	rBV3	1199	656	0.03%	0.004%
19	5.067	1143	1159	1178	rVV	325259	716916	37.87%	4.801%
20	5.170	1189	1191	1194	rVB3	1359	646	0.03%	0.004%
21	5.340	1241	1244	1247	rBV5	661	531	0.03%	0.004%
22	5.391	1257	1260	1266	rVV5	1182	1196	0.06%	0.008%
23	5.449	1274	1278	1281	rBV5	913	810	0.04%	0.005%
24	5.501	1291	1294	1296	rBV4	819	586	0.03%	0.004%
25	5.613	1326	1329	1338	rBV9	655	668	0.04%	0.004%
26	5.729	1341	1365	1394	rBV2	696361	1893041	100.00%	12.678%
27	5.964	1436	1438	1441	rBV3	982	699	0.04%	0.005%
28	5.999	1447	1449	1455	rVB6	1308	1173	0.06%	0.008%
29	6.031	1455	1459	1460	rBV4	1161	761	0.04%	0.005%
30	6.112	1480	1484	1487	rVV4	980	916	0.05%	0.006%
31	6.250	1513	1527	1558	rVV	524197	1017745	53.76%	6.816%
32	6.543	1605	1618	1627	rBV	6459	16196	0.86%	0.108%
33	6.694	1649	1665	1685	rBV	437251	856157	45.23%	5.734%
34	6.941	1741	1742	1747	rVB5	941	528	0.03%	0.004%
35	7.006	1760	1762	1768	rVB6	815	560	0.03%	0.004%
36	7.038	1768	1772	1773	rBV4	1040	617	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047119.D
 Acq On : 11 Feb 2022 16:46
 Operator : SY/MD
 Sample : N1474-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	7.186	1809	1818	1828	rVV8	2776	5484	0.29%	0.037%
38	7.362	1868	1873	1878	rVB6	1102	1235	0.07%	0.008%
39	7.401	1883	1885	1892	rVB8	898	703	0.04%	0.005%
40	7.443	1896	1898	1902	rVB5	894	612	0.03%	0.004%
41	7.469	1902	1906	1910	rBV6	977	885	0.05%	0.006%
42	7.568	1922	1937	1957	rBV	279423	493110	26.05%	3.302%
43	7.684	1969	1973	1983	rVB9	2709	4024	0.21%	0.027%
44	7.758	1994	1996	2004	rVB7	638	738	0.04%	0.005%
45	7.790	2004	2006	2009	rBV4	1390	766	0.04%	0.005%
46	7.899	2027	2040	2058	rBV	858040	1582376	83.59%	10.597%
47	8.179	2116	2127	2146	rBV	194780	326805	17.26%	2.189%
48	8.308	2165	2167	2169	rBV3	907	523	0.03%	0.004%
49	8.446	2207	2210	2212	rBV4	941	576	0.03%	0.004%
50	8.555	2236	2244	2255	rVB4	7864	12013	0.63%	0.080%
51	8.632	2255	2268	2282	rBV	724451	1222017	64.55%	8.184%
52	8.899	2346	2351	2354	rBV7	1216	1086	0.06%	0.007%
53	9.202	2440	2445	2448	rBV5	1022	704	0.04%	0.005%
54	9.343	2486	2489	2492	rVB4	801	610	0.03%	0.004%
55	9.369	2493	2497	2499	rBV6	886	618	0.03%	0.004%
56	9.420	2499	2513	2534	rBV	690865	1221548	64.53%	8.181%
57	9.565	2551	2558	2561	rBV8	1136	1514	0.08%	0.010%
58	9.697	2592	2599	2603	rBV6	2346	2846	0.15%	0.019%
59	9.954	2676	2679	2685	rBV7	723	715	0.04%	0.005%
60	10.047	2704	2708	2710	rBV4	841	575	0.03%	0.004%
61	10.066	2711	2714	2718	rVB5	1138	713	0.04%	0.005%
62	10.092	2719	2722	2725	rBV6	816	720	0.04%	0.005%
63	10.224	2760	2763	2768	rBV7	722	921	0.05%	0.006%
64	10.671	2896	2902	2910	rVB3	4745	6351	0.34%	0.043%
65	10.758	2913	2929	2953	rBV	610839	997941	52.72%	6.683%
66	10.967	2992	2994	2998	rBV5	899	700	0.04%	0.005%
67	11.201	3063	3067	3073	rVB7	907	869	0.05%	0.006%
68	11.301	3094	3098	3105	rVB8	1038	1248	0.07%	0.008%
69	11.337	3105	3109	3112	rBV4	822	598	0.03%	0.004%
70	11.417	3130	3134	3137	rBV7	1170	1096	0.06%	0.007%
71	11.462	3140	3148	3161	rVB7	4369	8645	0.46%	0.058%
72	11.510	3161	3163	3167	rVB4	833	560	0.03%	0.004%
73	11.555	3175	3177	3179	rBV3	853	536	0.03%	0.004%
74	11.700	3212	3222	3231	rBV8	2508	5266	0.28%	0.035%
75	11.812	3245	3257	3276	rBV	773078	1246587	65.85%	8.348%
76	12.037	3322	3327	3328	rBV4	724	697	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047119.D
 Acq On : 11 Feb 2022 16:46
 Operator : SY/MD
 Sample : N1474-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	12.192	3360	3375	3396	rVV	896723	1453932	76.80%	9.737%
78	12.327	3413	3417	3427	rBV10	1785	2830	0.15%	0.019%
79	12.391	3433	3437	3441	rBV6	1301	1426	0.08%	0.010%
80	12.455	3454	3457	3462	rBV6	920	663	0.04%	0.004%
81	12.719	3533	3539	3543	rBV6	844	898	0.05%	0.006%
82	12.771	3550	3555	3558	rBV5	1309	1430	0.08%	0.010%
83	12.899	3593	3595	3599	rBV4	813	670	0.04%	0.004%
84	13.163	3674	3677	3681	rVB4	891	598	0.03%	0.004%
85	13.462	3763	3770	3776	rBV5	1507	2421	0.13%	0.016%
86	13.500	3778	3782	3784	rBV5	782	584	0.03%	0.004%
87	13.825	3880	3883	3886	rBV5	1024	778	0.04%	0.005%
88	13.970	3924	3928	3929	rBV2	800	536	0.03%	0.004%
89	14.015	3938	3942	3944	rVB3	984	711	0.04%	0.005%
90	14.237	4008	4011	4015	rBV4	845	792	0.04%	0.005%
91	14.295	4026	4029	4032	rBV4	917	725	0.04%	0.005%
92	14.417	4064	4067	4070	rVB3	949	615	0.03%	0.004%
93	14.455	4075	4079	4081	rBV5	600	509	0.03%	0.003%
94	14.500	4090	4093	4096	rBV5	938	659	0.03%	0.004%
95	14.578	4112	4117	4119	rBV6	811	843	0.04%	0.006%
96	14.754	4168	4172	4176	rBV5	1188	1280	0.07%	0.009%
97	14.960	4230	4236	4239	rBV7	1036	1314	0.07%	0.009%
98	15.156	4292	4297	4302	rBV8	1219	1590	0.08%	0.011%
99	15.240	4319	4323	4324	rBV3	1197	916	0.05%	0.006%
100	15.549	4417	4419	4424	rVB4	1227	774	0.04%	0.005%




Sum of corrected areas: 14932099

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047119.D
Acq On : 11 Feb 2022 16:46
Operator : SY/MD
Sample : N1474-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

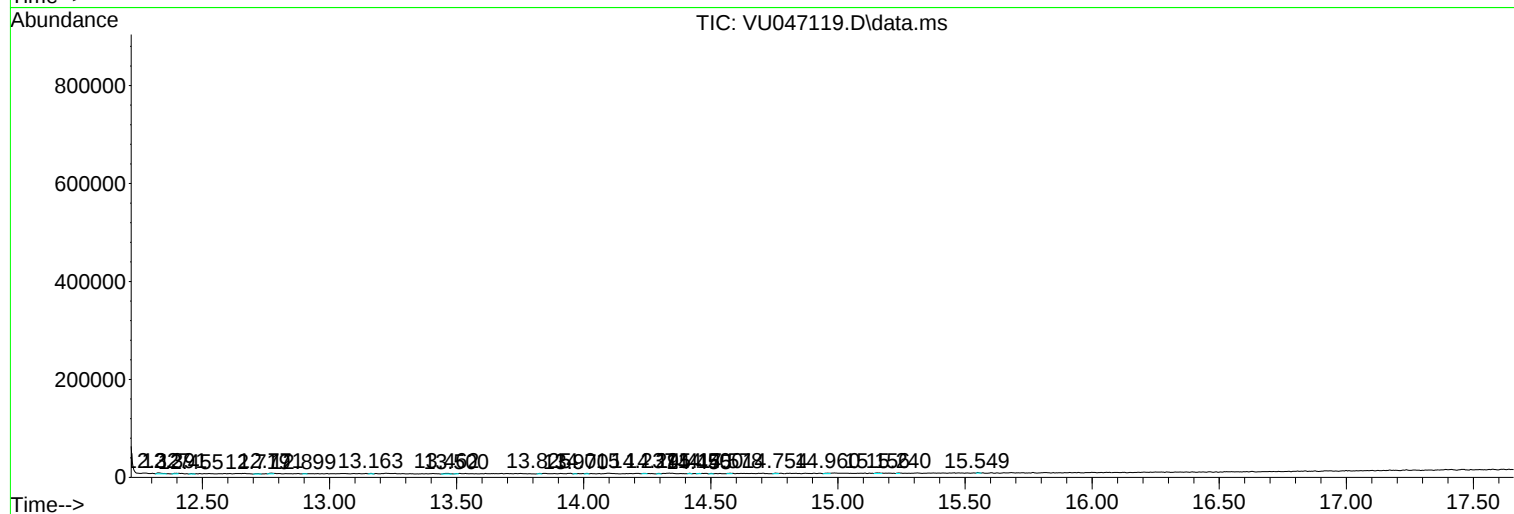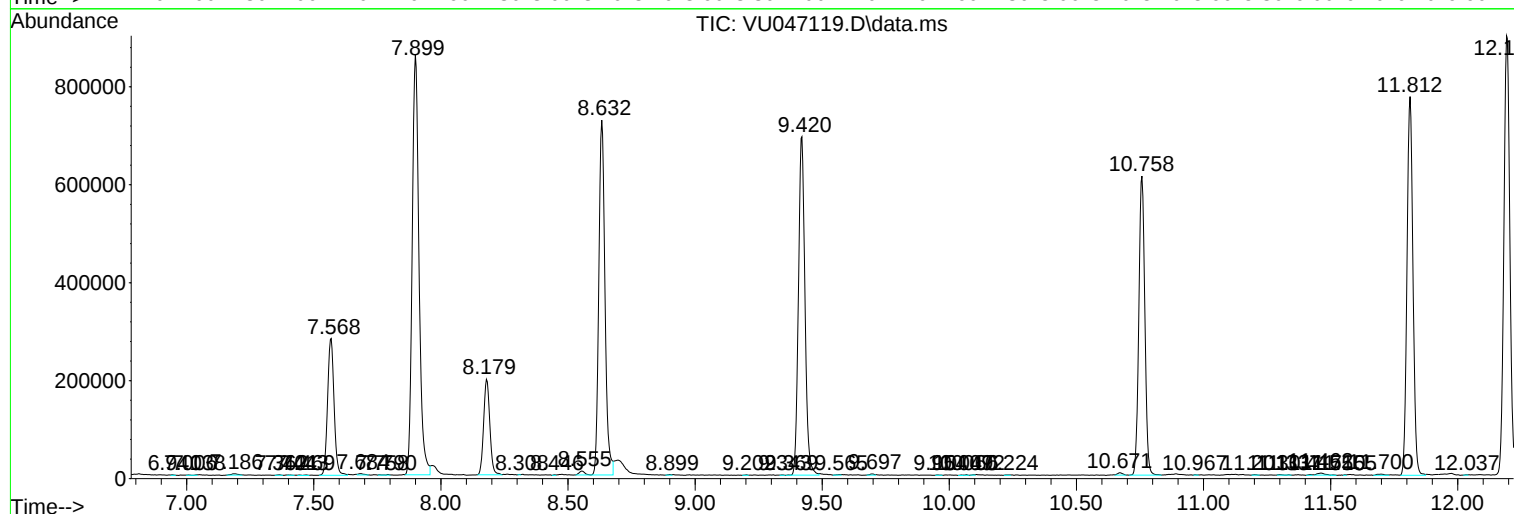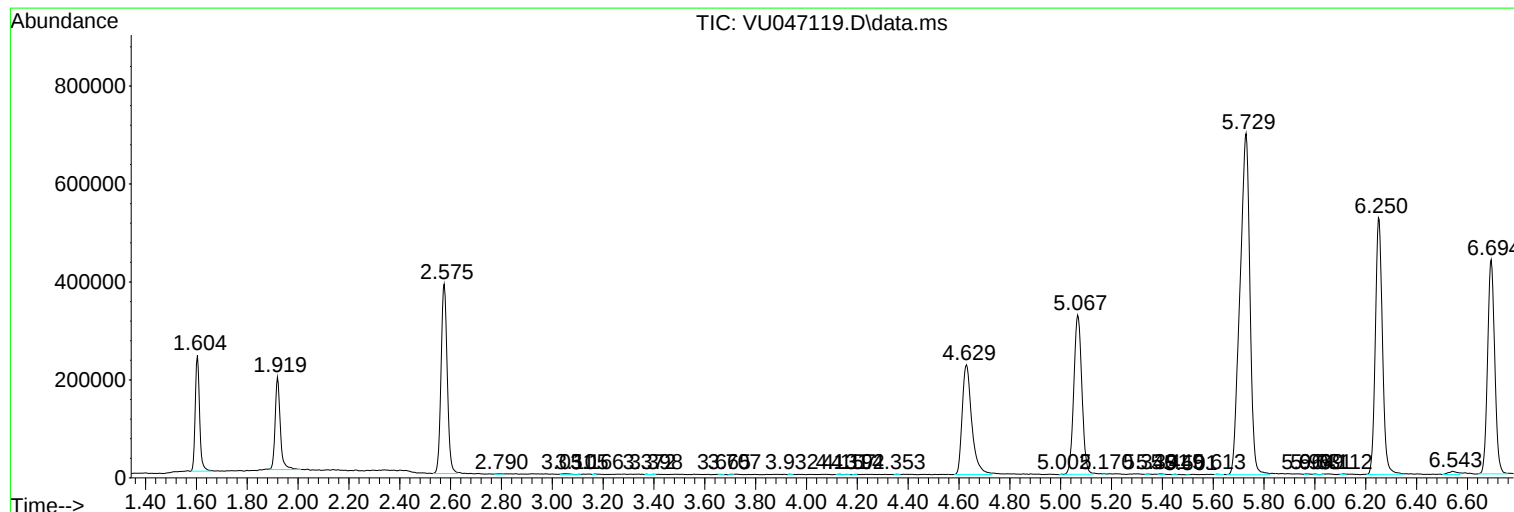

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047119.D
Acq On : 11 Feb 2022 16:46
Operator : SY/MD
Sample : N1474-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047119.D
Acq On : 11 Feb 2022 16:46
Operator : SY/MD
Sample : N1474-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc