

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047120.D
 Acq On : 11 Feb 2022 17:09
 Operator : SY/MD
 Sample : N1462-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	103	rVB	214379	253715	13.55%	1.699%
2	1.919	172	180	207	rVB	177583	253271	13.53%	1.696%
3	2.575	371	384	402	rBV	365591	611822	32.68%	4.097%
4	2.719	426	429	432	rBV4	924	686	0.04%	0.005%
5	2.941	495	498	501	rBV3	1048	807	0.04%	0.005%
6	2.961	501	504	507	rVV5	894	796	0.04%	0.005%
7	3.041	522	529	531	rBV6	1610	1526	0.08%	0.010%
8	3.108	547	550	554	rBV6	646	548	0.03%	0.004%
9	3.321	614	616	619	rBV4	724	560	0.03%	0.004%
10	3.369	625	631	638	rBV9	1283	1802	0.10%	0.012%
11	3.600	699	703	707	rBV5	973	886	0.05%	0.006%
12	3.642	712	716	718	rBV5	697	565	0.03%	0.004%
13	3.906	796	798	802	rVB3	1095	648	0.03%	0.004%
14	3.973	814	819	821	rBV4	772	647	0.03%	0.004%
15	4.041	836	840	841	rBV4	838	545	0.03%	0.004%
16	4.137	866	870	871	rVV3	889	728	0.04%	0.005%
17	4.147	871	873	878	rVB6	1296	1011	0.05%	0.007%
18	4.176	878	882	886	rBV7	1028	811	0.04%	0.005%
19	4.202	886	890	893	rVV4	710	606	0.03%	0.004%
20	4.517	984	988	991	rBV4	717	642	0.03%	0.004%
21	4.626	1007	1022	1053	rBV	245946	622308	33.24%	4.167%
22	4.935	1114	1118	1123	rVB7	789	728	0.04%	0.005%
23	5.067	1143	1159	1182	rBV	326767	716462	38.27%	4.798%
24	5.198	1194	1200	1202	rBV7	1055	1027	0.05%	0.007%
25	5.234	1209	1211	1216	rVB6	1123	739	0.04%	0.005%
26	5.292	1224	1229	1232	rBV7	920	1010	0.05%	0.007%
27	5.340	1242	1244	1249	rVB4	989	584	0.03%	0.004%
28	5.452	1277	1279	1284	rVB5	1119	830	0.04%	0.006%
29	5.729	1339	1365	1386	rBV2	680295	1872263	100.00%	12.537%
30	6.057	1465	1467	1476	rVB8	1179	1149	0.06%	0.008%
31	6.253	1509	1528	1561	rBV	505206	1005980	53.73%	6.736%
32	6.436	1581	1585	1587	rBV3	756	586	0.03%	0.004%
33	6.513	1602	1609	1610	rVB6	1566	1462	0.08%	0.010%
34	6.546	1610	1619	1622	rBV8	3814	6356	0.34%	0.043%
35	6.694	1650	1665	1685	rBV	432822	853208	45.57%	5.713%
36	6.957	1743	1747	1751	rVB5	1376	1137	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047120.D
 Acq On : 11 Feb 2022 17:09
 Operator : SY/MD
 Sample : N1462-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	6.983	1751	1755	1758	rBV5	1100	858	0.05%	0.006%
38	7.047	1764	1775	1780	rBV9	1598	2218	0.12%	0.015%
39	7.089	1785	1788	1794	rBV6	738	604	0.03%	0.004%
40	7.128	1798	1800	1809	rVB7	850	1058	0.06%	0.007%
41	7.189	1809	1819	1827	rBV7	4110	9213	0.49%	0.062%
42	7.247	1832	1837	1841	rBV7	761	618	0.03%	0.004%
43	7.343	1863	1867	1870	rVB4	818	650	0.03%	0.004%
44	7.369	1870	1875	1879	rBV5	862	1121	0.06%	0.008%
45	7.443	1895	1898	1903	rVB5	631	547	0.03%	0.004%
46	7.485	1906	1911	1913	rBV5	965	602	0.03%	0.004%
47	7.568	1924	1937	1955	rBV	279108	490248	26.18%	3.283%
48	7.790	2002	2006	2007	rBV4	918	600	0.03%	0.004%
49	7.899	2026	2040	2059	rBV	835608	1556810	83.15%	10.425%
50	8.083	2095	2097	2101	rVB4	1296	869	0.05%	0.006%
51	8.179	2114	2127	2147	rBV	196523	334393	17.86%	2.239%
52	8.327	2171	2173	2177	rVB3	1597	1019	0.05%	0.007%
53	8.549	2237	2242	2253	rVB3	3709	6193	0.33%	0.041%
54	8.632	2254	2268	2284	rBV	760337	1314364	70.20%	8.802%
55	8.909	2350	2354	2356	rBV4	1595	1148	0.06%	0.008%
56	9.221	2446	2451	2454	rBV5	700	757	0.04%	0.005%
57	9.292	2467	2473	2476	rBV6	796	956	0.05%	0.006%
58	9.420	2497	2513	2537	rBV	675301	1210261	64.64%	8.104%
59	9.571	2555	2560	2571	rBV8	1409	2243	0.12%	0.015%
60	9.697	2592	2599	2608	rVB7	2739	4524	0.24%	0.030%
61	9.803	2627	2632	2635	rBV5	1168	1085	0.06%	0.007%
62	9.848	2643	2646	2648	rBV4	859	653	0.03%	0.004%
63	9.877	2652	2655	2658	rBV4	868	655	0.03%	0.004%
64	9.941	2672	2675	2679	rVB5	703	536	0.03%	0.004%
65	9.967	2679	2683	2689	rBV6	875	880	0.05%	0.006%
66	10.015	2695	2698	2704	rVB5	843	634	0.03%	0.004%
67	10.115	2723	2729	2734	rVB8	1459	1885	0.10%	0.013%
68	10.224	2757	2763	2764	rBV7	617	635	0.03%	0.004%
69	10.263	2770	2775	2778	rVB5	824	609	0.03%	0.004%
70	10.433	2825	2828	2832	rBV6	707	685	0.04%	0.005%
71	10.491	2843	2846	2850	rVB5	1171	822	0.04%	0.006%
72	10.526	2854	2857	2864	rVB5	1318	1123	0.06%	0.008%
73	10.671	2893	2902	2913	rVV3	4009	6877	0.37%	0.046%
74	10.758	2915	2929	2948	rVV	635545	1027319	54.87%	6.879%
75	11.018	3007	3010	3015	rVB6	831	719	0.04%	0.005%
76	11.063	3022	3024	3028	rVB3	988	674	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047120.D
 Acq On : 11 Feb 2022 17:09
 Operator : SY/MD
 Sample : N1462-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	11.095	3028	3034	3038	rBV7	1714	2213	0.12%	0.015%
78	11.275	3087	3090	3093	rBV4	1125	992	0.05%	0.007%
79	11.414	3129	3133	3137	rBV6	1583	1606	0.09%	0.011%
80	11.462	3143	3148	3161	rVB9	4620	7957	0.42%	0.053%
81	11.517	3161	3165	3170	rBV8	658	627	0.03%	0.004%
82	11.677	3211	3215	3216	rBV4	1111	664	0.04%	0.004%
83	11.751	3231	3238	3242	rVB7	1373	1451	0.08%	0.010%
84	11.812	3244	3257	3282	rVV	774148	1232618	65.84%	8.254%
85	12.192	3360	3375	3396	rBV	898697	1465425	78.27%	9.813%
86	12.455	3454	3457	3461	rVB5	904	635	0.03%	0.004%
87	12.529	3476	3480	3483	rBV6	1046	926	0.05%	0.006%
88	12.687	3527	3529	3534	rVB2	867	557	0.03%	0.004%
89	12.774	3549	3556	3563	rVB5	1872	2868	0.15%	0.019%
90	13.108	3656	3660	3663	rVB5	901	721	0.04%	0.005%
91	13.137	3664	3669	3670	rBV4	754	631	0.03%	0.004%
92	13.298	3713	3719	3723	rVB8	677	928	0.05%	0.006%
93	13.732	3848	3854	3857	rBV7	745	739	0.04%	0.005%
94	13.844	3884	3889	3894	rVV5	1219	1603	0.09%	0.011%
95	14.057	3952	3955	3957	rBV2	700	582	0.03%	0.004%
96	14.073	3957	3960	3962	rBV4	974	669	0.04%	0.004%
97	14.230	4006	4009	4015	rBV8	779	697	0.04%	0.005%
98	14.494	4088	4091	4095	rBV6	750	606	0.03%	0.004%
99	14.574	4111	4116	4117	rBV3	1242	1001	0.05%	0.007%
100	14.809	4187	4189	4193	rVB5	789	552	0.03%	0.004%




Sum of corrected areas: 14933384

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047120.D
Acq On : 11 Feb 2022 17:09
Operator : SY/MD
Sample : N1462-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

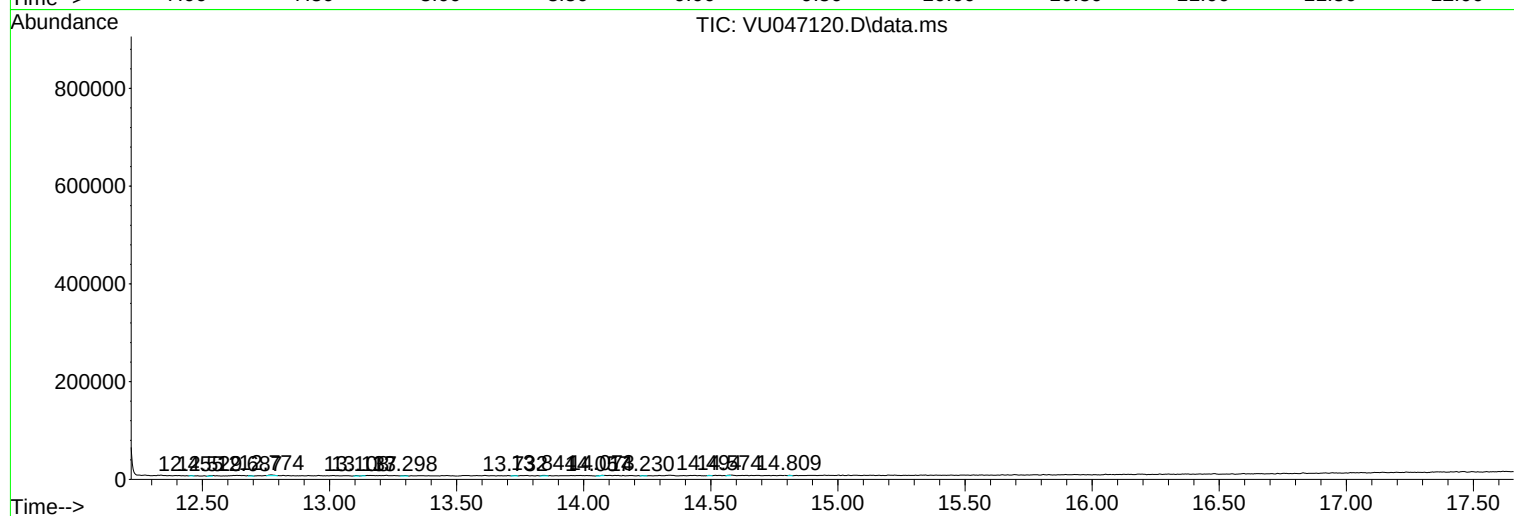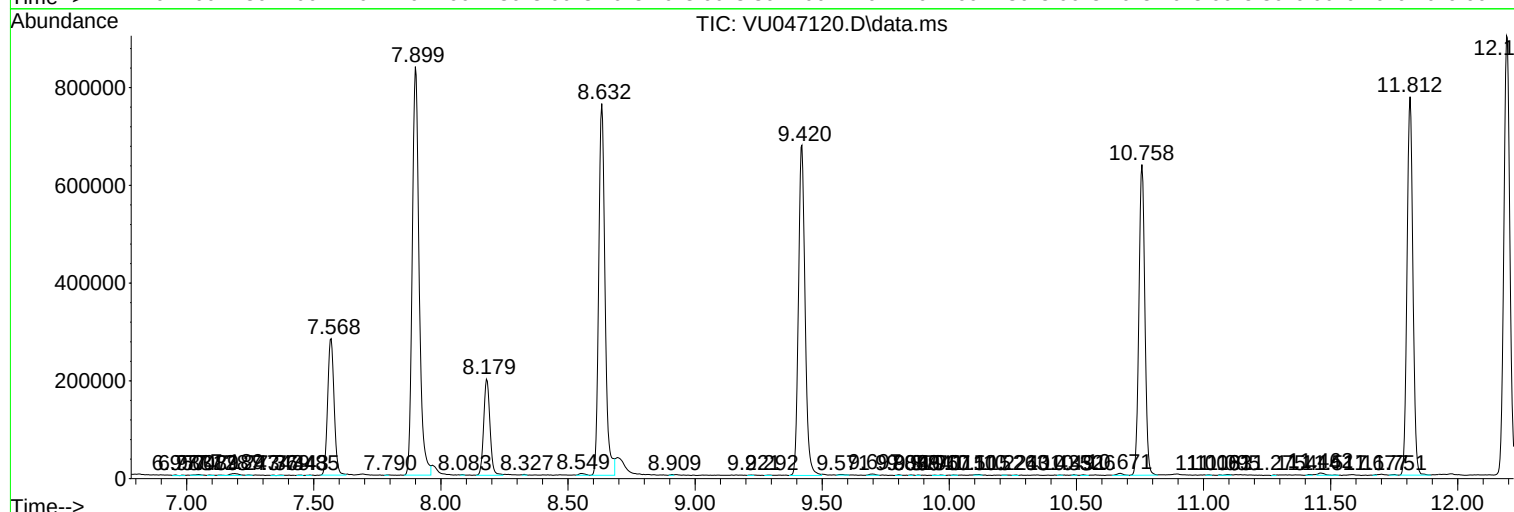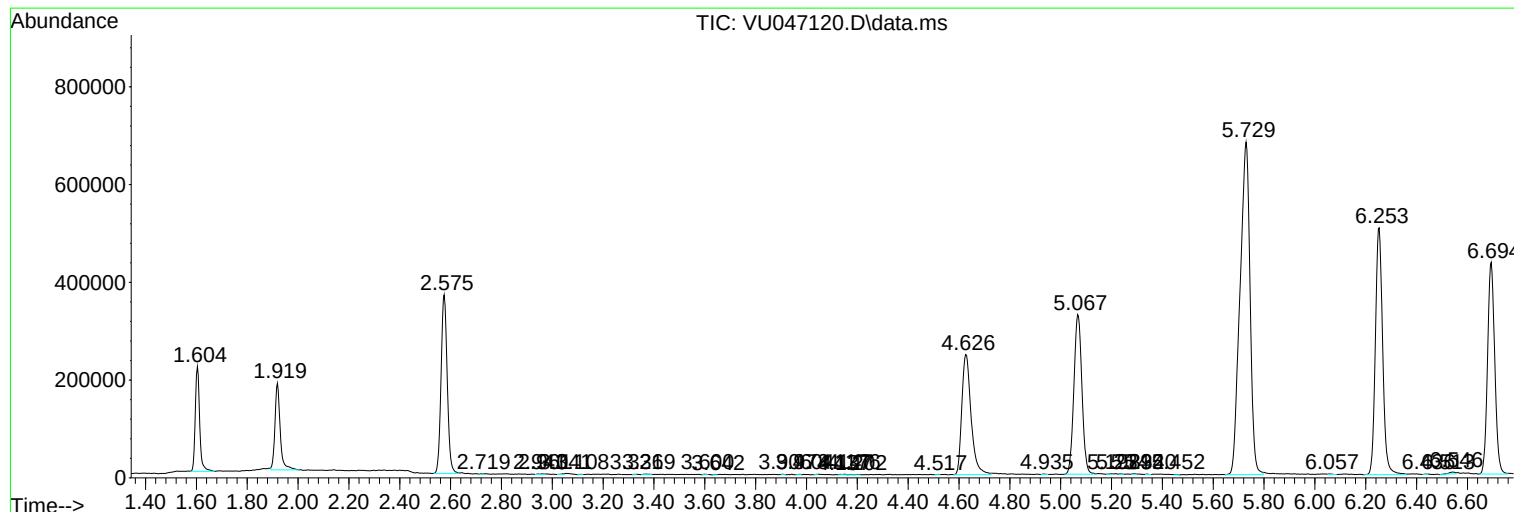

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047120.D
Acq On : 11 Feb 2022 17:09
Operator : SY/MD
Sample : N1462-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
Data File : VU047120.D
Acq On : 11 Feb 2022 17:09
Operator : SY/MD
Sample : N1462-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------