


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021122\
 Data File : VU047102.D
 Acq On : 11 Feb 2022 08:59
 Operator : SY/MD
 Sample : BFB044
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB044

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis
 Last Update : Fri Feb 18 00:54:38 2022

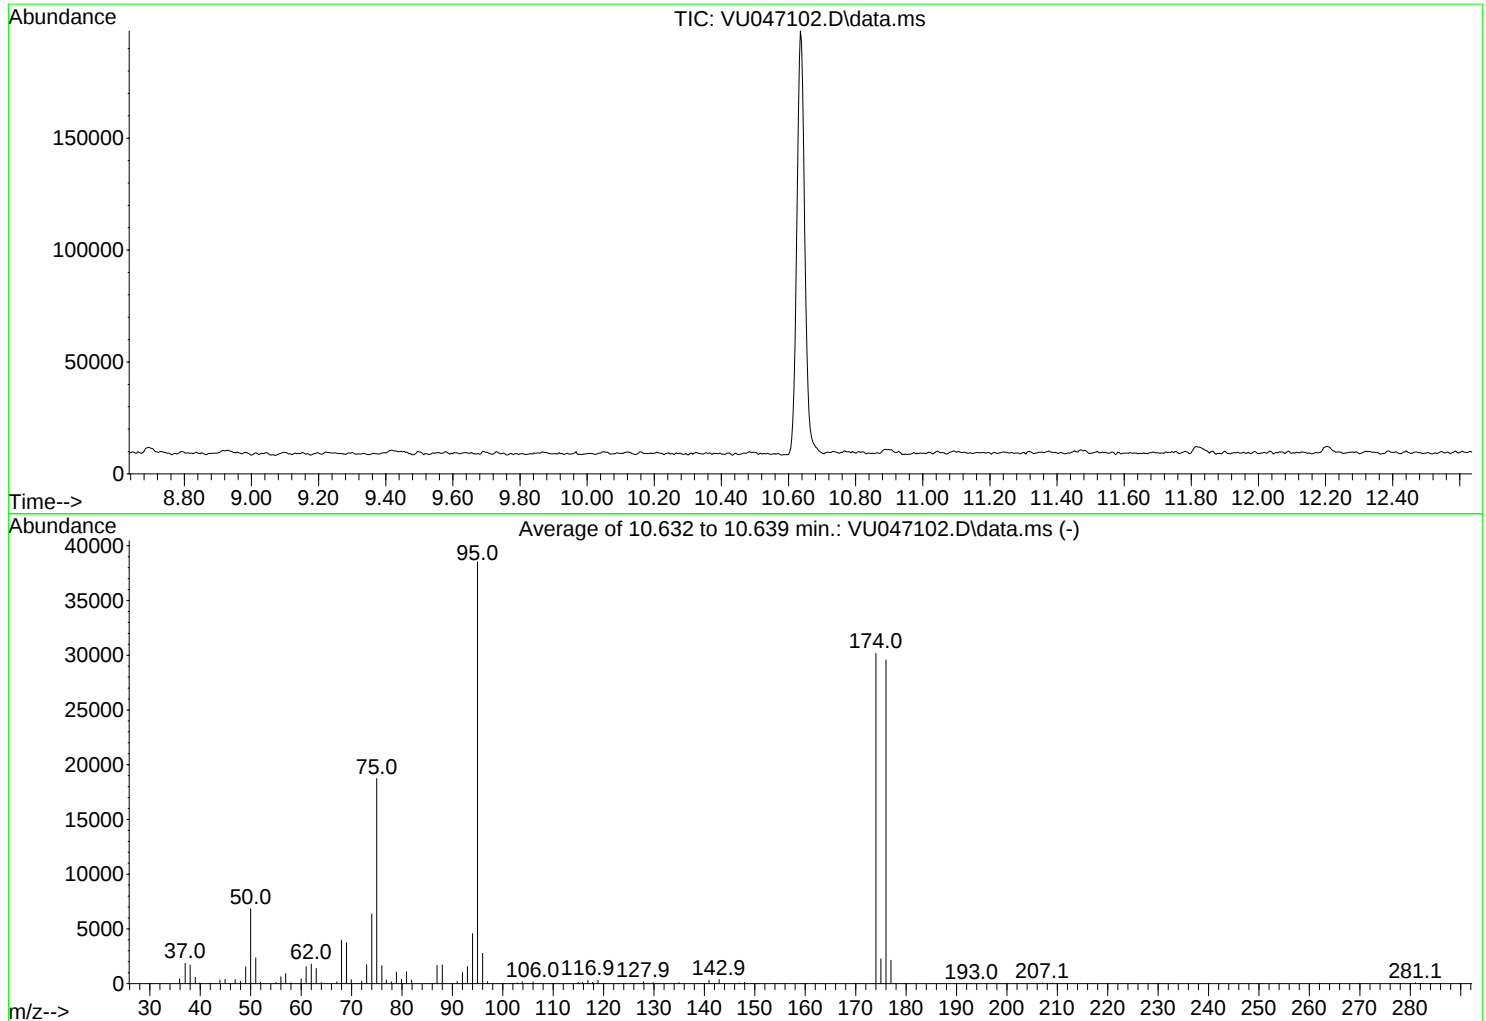

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	6840	PASS
75	95	30	80	48.6	18739	PASS
95	95	100	100	100.0	38531	PASS
96	95	5	9	7.2	2778	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.3	30173	PASS
175	174	5	9	7.5	2261	PASS
176	174	95	101	98.0	29573	PASS
177	176	5	9	7.2	2141	PASS

m/z	Abundance
39.00	234.0
39.80	147.0
41.10	234.0
42.10	138.0
42.90	360.0
44.00	777.0
44.90	177.0
55.00	211.0
56.00	100.0
56.90	127.0
69.10	107.0
73.00	277.0
75.00	112.0
96.00	371.0
133.00	372.0
146.90	102.0
191.00	304.0
193.00	114.0
207.10	3036.0
208.10	598.0
209.00	384.0
281.10	388.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.90	433.0
37.00	1857.0
38.00	1719.0
39.00	754.0
39.90	206.0
41.00	230.0
41.90	176.0
43.00	398.0
43.90	1103.0
45.00	533.0
46.90	347.0
48.00	222.0
49.00	1569.0
50.00	6673.0
51.00	2287.0
52.00	133.0
55.00	321.0
56.00	754.0
57.00	1063.0
58.00	119.0
60.00	410.0
61.00	1532.0
62.00	1774.0
63.00	1315.0
64.00	185.0
67.10	172.0
68.00	3852.0
69.00	3747.0
70.00	406.0
72.00	226.0
73.00	1947.0
74.00	6278.0
75.00	18424.0
76.00	1542.0
76.90	319.0
77.90	156.0
78.90	995.0
79.90	376.0
80.90	1015.0
81.90	319.0
87.00	1547.0
88.00	1588.0
90.90	219.0
92.00	994.0
93.00	1516.0
94.00	4436.0
95.00	37384.0
96.00	3199.0
97.00	180.0
103.90	170.0
106.00	123.0
115.00	115.0
115.80	146.0
116.90	281.0
117.80	127.0
118.90	286.0
127.90	162.0
133.00	282.0
135.00	103.0
140.90	302.0
142.90	367.0
147.10	154.0
147.90	108.0
174.00	28344.0
175.00	2160.0
176.00	27744.0
177.00	2056.0
191.00	234.0
193.00	143.0
207.00	3186.0
208.00	593.0
209.00	440.0
281.10	476.0
282.00	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.90	475.0
37.00	1918.0
38.00	1742.0
39.00	870.0
39.90	214.0
41.00	223.0
42.00	168.0
43.00	362.0
43.90	1117.0
45.00	574.0
46.90	393.0
47.90	226.0
49.00	1576.0
50.00	7025.0
51.00	2470.0
52.00	126.0
55.00	336.0
56.00	757.0
57.00	1073.0
58.00	104.0
60.00	460.0
61.00	1595.0
62.00	1845.0
63.00	1432.0
64.00	141.0
67.10	188.0
68.00	4099.0
69.00	3971.0
69.90	367.0
72.00	248.0
73.00	2068.0
74.00	6632.0
75.00	19432.0
76.00	1675.0
76.90	332.0
77.90	149.0
78.90	1095.0
79.90	416.0
80.90	1132.0
81.90	341.0
87.00	1726.0
88.00	1777.0
90.90	225.0
92.00	1057.0
93.00	1621.0
94.00	4714.0
95.00	39648.0
96.00	3254.0
97.00	179.0
102.80	112.0
103.90	180.0
106.00	154.0
114.90	114.0
115.80	138.0
116.90	317.0
117.80	126.0
118.90	305.0
127.90	182.0
129.90	146.0
133.00	244.0
134.90	107.0
140.90	307.0
142.90	399.0
147.00	172.0
147.90	117.0
174.00	31072.0
175.00	2330.0
176.00	30424.0
177.00	2200.0
191.00	278.0
193.00	135.0
207.10	3157.0
208.00	622.0
209.00	448.0
281.00	497.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.90	420.0
37.00	1823.0
38.00	1627.0
39.00	842.0
39.90	199.0
40.90	229.0
42.00	167.0
43.00	317.0
43.90	1068.0
44.90	571.0
46.90	401.0
47.90	232.0
49.00	1462.0
50.00	6822.0
51.00	2323.0
51.90	118.0
55.00	341.0
56.00	662.0
57.00	1030.0
60.00	466.0
61.00	1535.0
62.00	1727.0
63.00	1398.0
67.10	174.0
68.00	3919.0
69.00	3847.0
70.00	326.0
72.00	234.0
73.00	1985.0
74.00	6233.0
75.00	18696.0
76.00	1717.0
76.90	313.0
77.90	158.0
78.90	1092.0
79.90	405.0
80.90	1115.0
81.90	320.0
86.90	1741.0
88.00	1757.0
91.00	192.0
92.00	1041.0
93.00	1561.0
94.00	4515.0
95.00	38560.0
96.00	2995.0
97.00	196.0
102.90	116.0
103.80	183.0
106.00	192.0
114.90	119.0
115.90	117.0
116.90	317.0
117.80	108.0
118.90	298.0
127.90	192.0
129.80	174.0
133.00	234.0
134.90	102.0
140.90	293.0
142.90	367.0
147.00	164.0
148.00	121.0
174.00	31104.0
175.00	2292.0
176.00	30552.0
177.00	2166.0
191.00	329.0
193.00	129.0
207.10	2972.0
208.00	635.0
209.00	424.0
281.00	469.0
282.20	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044