


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021823\
Data File : VU053125.D
Acq On : 18 Feb 2023 10:46
Operator : JC/MD
Sample : BFB198
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB198

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021023WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sun Feb 19 23:26:18 2023

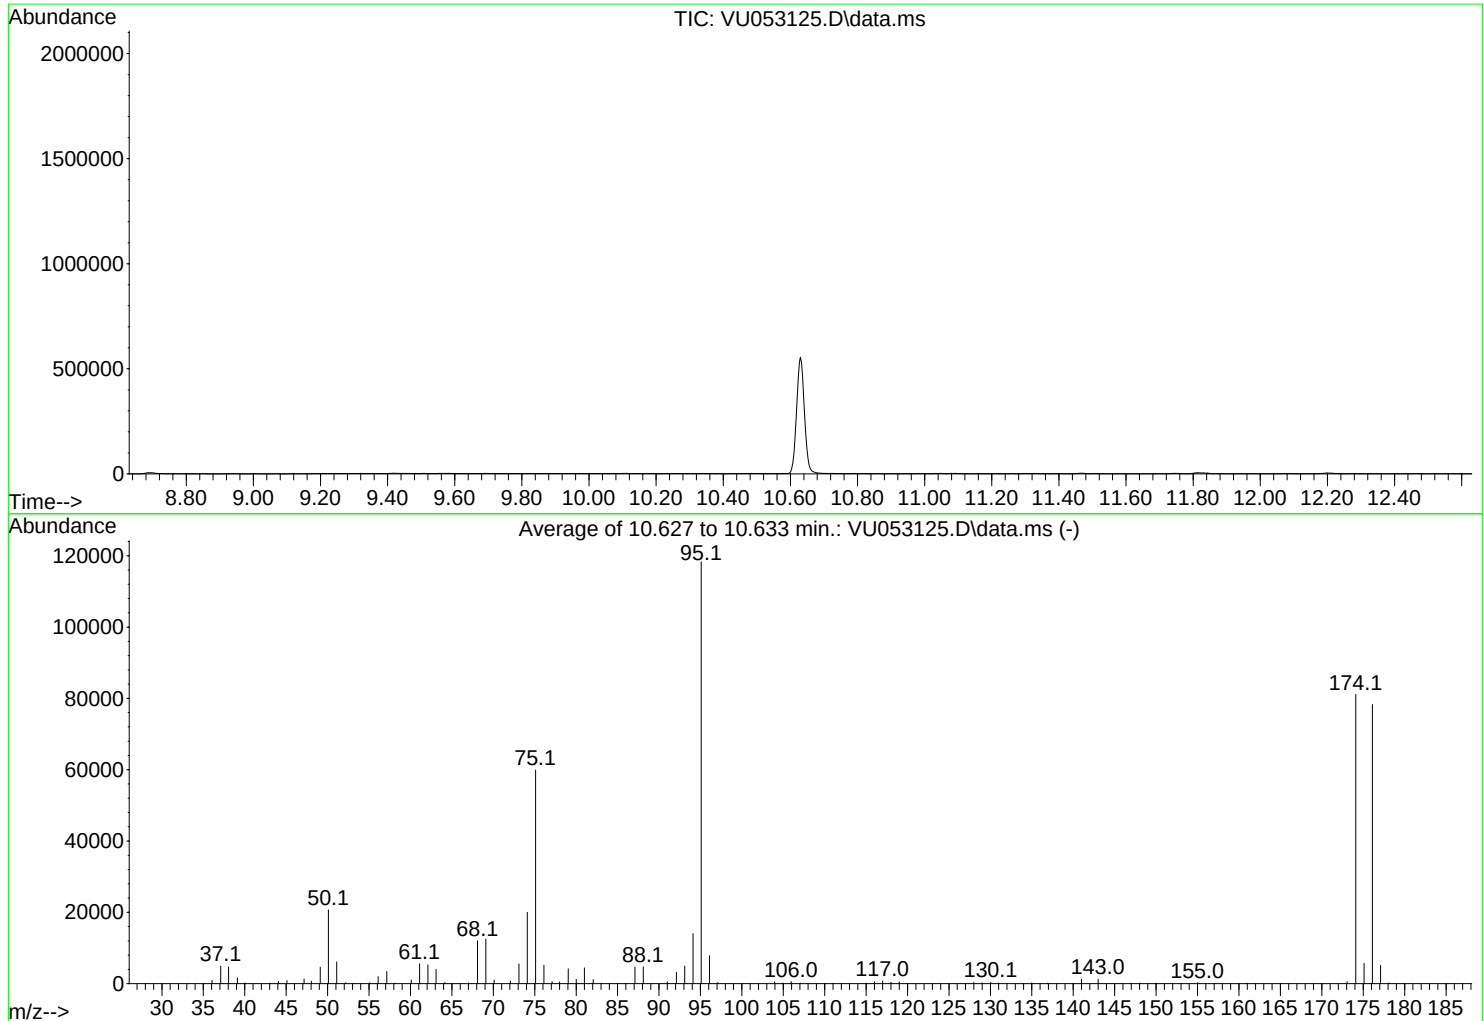

AutoFind: Scans 2966, 2967, 2968; Background Corrected with Scan 2952

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	20675	PASS
75	95	30	80	50.6	59915	PASS
95	95	100	100	100.0	118293	PASS
96	95	5	9	6.6	7841	PASS
173	174	0.00	2	0.7	533	PASS
174	95	50	120	68.6	81120	PASS
175	174	5	9	7.0	5700	PASS
176	174	95	101	96.5	78285	PASS
177	176	5	9	6.5	5108	PASS

m/z	Abundance
35.10	151.0
36.00	687.0
38.00	215.0
44.00	229.0
55.10	141.0
57.20	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB198

m/z	Abundance
35.10	104.0
36.10	1583.0
37.10	4978.0
38.10	4742.0
39.10	1641.0
40.00	184.0
43.10	107.0
44.10	985.0
45.10	863.0
47.20	1386.0
48.10	674.0
49.10	4480.0
50.10	20584.0
51.10	6315.0
52.20	294.0
55.10	369.0
56.10	1876.0
57.20	3607.0
58.10	148.0
60.10	1071.0
61.10	5478.0
62.10	5368.0
63.10	3993.0
64.10	405.0
67.00	290.0
68.10	11882.0
69.10	12957.0
70.10	915.0
72.10	778.0
73.10	5529.0
74.10	20048.0
75.10	59728.0
76.10	5316.0
77.10	595.0
78.00	481.0
79.00	4131.0
80.00	1174.0
81.00	4263.0
82.00	1157.0
83.10	155.0
86.10	119.0
87.10	4495.0
88.10	4741.0
91.00	514.0
92.10	3145.0
93.10	4909.0
94.10	14033.0
95.10	116872.0
96.10	8044.0
97.10	321.0
103.90	537.0
105.00	201.0
106.00	561.0
107.10	113.0
111.00	104.0
115.00	118.0
116.00	489.0
117.00	807.0
118.00	379.0
119.00	487.0
128.00	378.0
129.00	202.0
130.00	416.0
131.00	176.0
135.00	232.0
136.90	106.0
141.00	1243.0
143.00	1130.0
146.90	107.0
148.00	172.0
150.00	127.0
155.00	280.0
157.00	185.0
161.00	117.0
173.00	515.0
174.10	77976.0
175.10	5595.0
176.10	75176.0
177.10	4932.0
178.10	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB198

m/z	Abundance
36.10	1696.0
37.10	5129.0
38.10	5025.0
39.10	1623.0
40.00	158.0
43.10	127.0
44.10	882.0
45.10	875.0
47.20	1366.0
48.00	692.0
49.10	4779.0
50.10	21208.0
51.10	6224.0
52.20	316.0
55.10	441.0
56.10	2071.0
57.10	3638.0
58.10	163.0
60.10	1065.0
61.10	5762.0
62.10	5366.0
63.10	4190.0
64.20	292.0
67.00	240.0
68.10	12398.0
69.10	12971.0
70.10	986.0
72.10	779.0
73.10	5729.0
74.10	20704.0
75.10	61632.0
76.10	5363.0
77.10	597.0
78.00	481.0
79.00	4311.0
80.00	1244.0
81.00	4569.0
82.00	1149.0
83.10	116.0
87.10	4818.0
88.10	4935.0
91.00	515.0
92.10	3265.0
93.10	5055.0
94.10	14432.0
95.10	122280.0
96.10	8121.0
97.10	333.0
103.90	551.0
105.00	198.0
105.90	626.0
107.10	139.0
115.00	118.0
116.00	488.0
117.00	784.0
118.00	429.0
119.00	480.0
128.00	394.0
129.00	263.0
130.00	426.0
131.00	214.0
135.00	254.0
136.90	118.0
141.00	1299.0
143.00	1295.0
146.90	100.0
148.10	175.0
150.00	138.0
153.00	107.0
155.00	314.0
157.00	141.0
161.00	159.0
173.00	550.0
174.10	83848.0
175.10	5869.0
176.10	80808.0
177.10	5244.0
178.10	212.0

Instrument :
MSVOA_U
ClientSampleId :
BFB198

m/z	Abundance
36.10	1614.0
37.10	4728.0
38.10	4848.0
39.10	1585.0
40.10	140.0
43.10	131.0
44.10	749.0
45.10	825.0
47.10	1199.0
48.00	685.0
49.10	4558.0
50.10	20232.0
51.10	5788.0
52.20	289.0
55.10	465.0
56.10	1931.0
57.10	3315.0
58.20	145.0
60.10	1014.0
61.10	5478.0
62.10	5097.0
63.10	3827.0
64.20	236.0
67.00	170.0
68.10	11797.0
69.10	11682.0
70.10	1003.0
72.00	656.0
73.10	5372.0
74.10	19360.0
75.10	58384.0
76.10	4740.0
77.10	575.0
78.00	465.0
79.10	4097.0
80.00	1169.0
81.00	4445.0
82.10	1061.0
83.00	106.0
87.10	4652.0
88.10	4502.0
91.00	476.0
92.10	3129.0
93.10	4846.0
94.10	13730.0
95.10	115728.0
96.10	7358.0
97.10	299.0
104.00	465.0
104.90	173.0
105.90	602.0
107.00	137.0
111.00	114.0
112.00	104.0
115.00	112.0
116.00	473.0
117.00	705.0
118.00	424.0
119.00	466.0
128.00	368.0
129.00	266.0
130.10	374.0
131.00	201.0
135.00	238.0
136.90	138.0
141.00	1197.0
143.00	1343.0
145.90	108.0
148.00	179.0
150.00	132.0
155.00	282.0
160.90	173.0
173.10	534.0
174.10	81536.0
175.10	5635.0
176.10	78872.0
177.10	5149.0
178.10	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB198