

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061622\
 Data File : VU049199.D
 Acq On : 16 Jun 2022 11:56
 Operator : SY/MD
 Sample : N3278-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BF9

Quant Time: Jun 17 01:26:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 17 01:23:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	125800	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	113086	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	55785	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	41975	3.819	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	76.400%	
7) Chloroethane-d5	1.912	69	32818	4.410	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	88.200%	
11) 1,1-Dichloroethene-d2	2.565	65	17307	3.914	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	78.200%	
20) 2-Butanone-d5	4.636	46	151407	51.587	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.180%	
24) Chloroform-d	5.067	84	78009	4.523	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.400%	
26) 1,2-Dichloroethane-d4	5.703	65	44471	4.701	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.000%	
32) Benzene-d6	5.729	84	159100	4.670	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.400%	
36) 1,2-Dichloropropane-d6	6.694	67	55786	4.825	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.400%	
41) Toluene-d8	7.899	98	139984	4.563	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.200%	
43) trans-1,3-Dichloroprop...	8.179	79	18786	3.657	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	73.200%	
46) 2-Hexanone-d5	8.636	63	96880	46.753	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	93.500%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	43892	4.741	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.800%	
66) 1,2-Dichlorobenzene-d4	12.192	152	51453	4.807	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.200%	
Target Compounds						
					Qvalue	
13) Acetone	2.649	43	77188	53.138	ug/L	97
21) 2-Butanone	4.719	43	12261	4.427	ug/L	91
53) m,p-Xylene	9.693	106	1475	0.102	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061622\
Data File : VU049199.D
Acq On : 16 Jun 2022 11:56
Operator : SY/MD
Sample : N3278-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BF9

Quant Time: Jun 17 01:26:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 17 01:23:56 2022
Response via : Initial Calibration




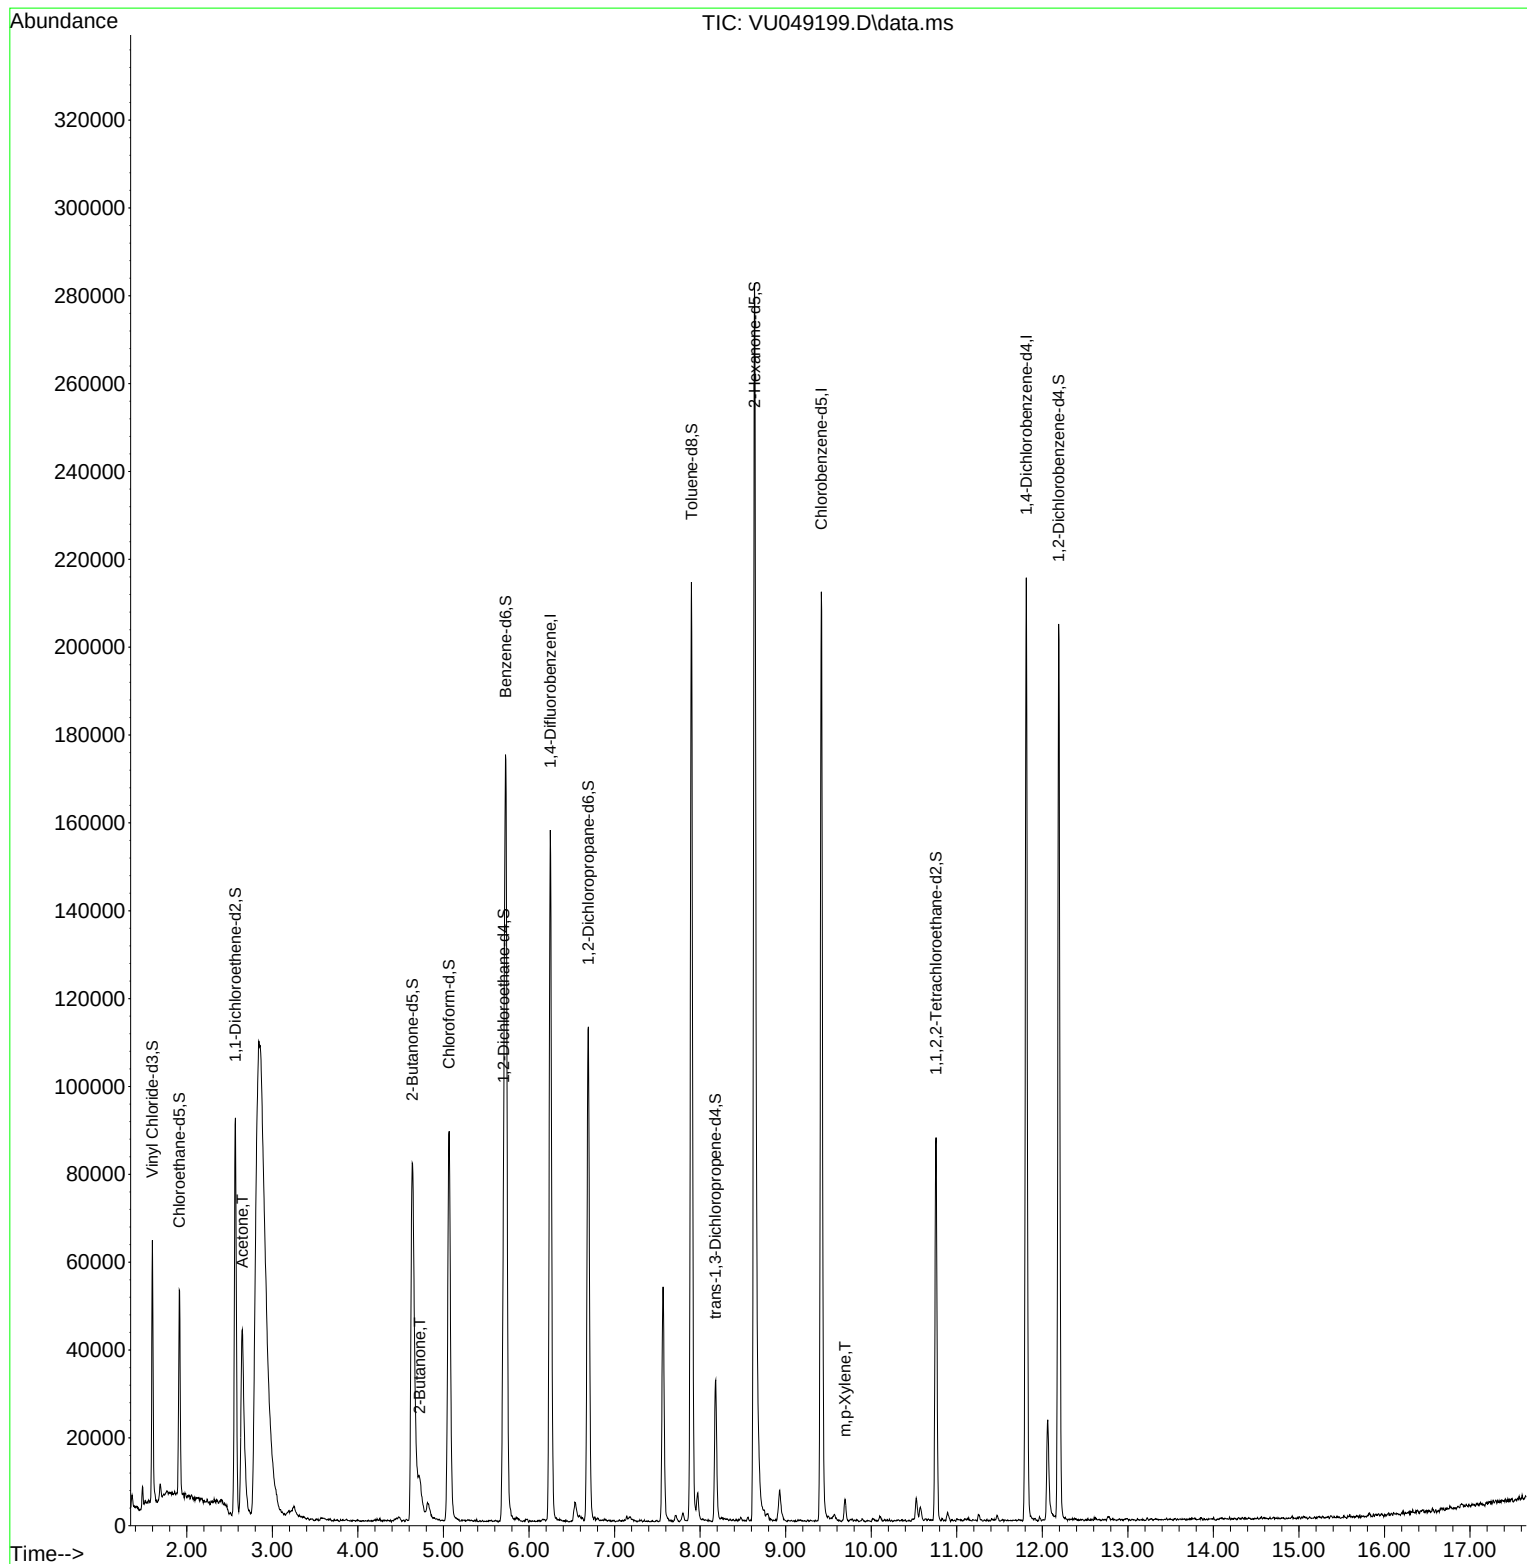


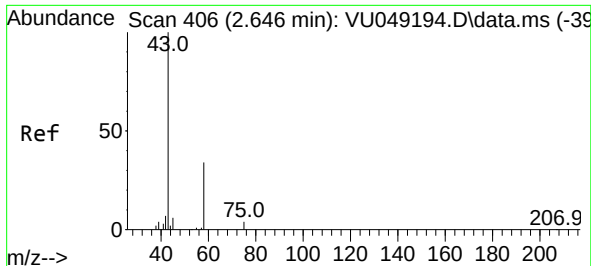

#13
Acetone
Concen: 53.138 ug/L
RT: 2.649 min Scan# 406
Delta R.T. 0.003 min
Lab File: VU049199.D
Acq: 16 Jun 2022 11:56




Instrument :
MSVOA_U
ClientSampleId :
C0BF9


Tgt Ion: 43 Resp: 77188
Ion Ratio Lower Upper
43 100
58 31.3 0.0 65.8

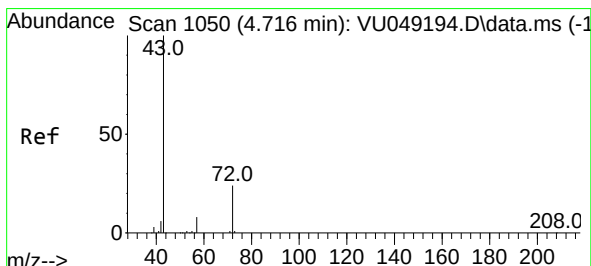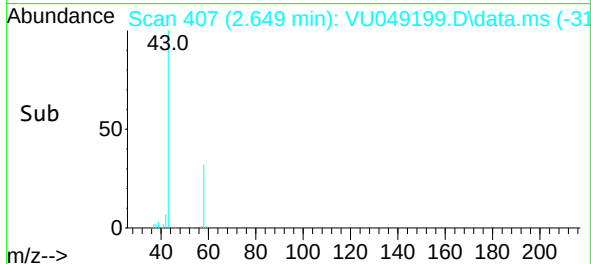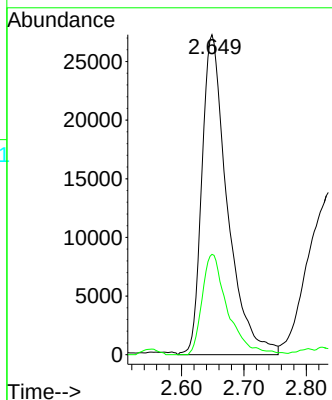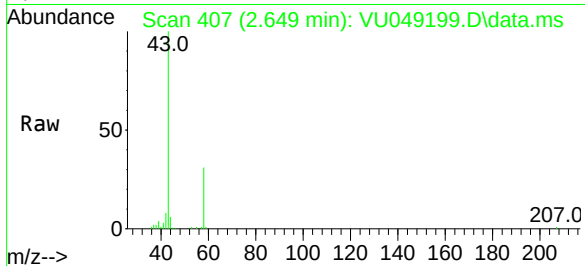

#21
2-Butanone
Concen: 4.427 ug/L
RT: 4.719 min Scan# 1051
Delta R.T. 0.003 min
Lab File: VU049199.D
Acq: 16 Jun 2022 11:56


Tgt Ion: 43 Resp: 12261
Ion Ratio Lower Upper
43 100
72 20.1 12.2 36.6

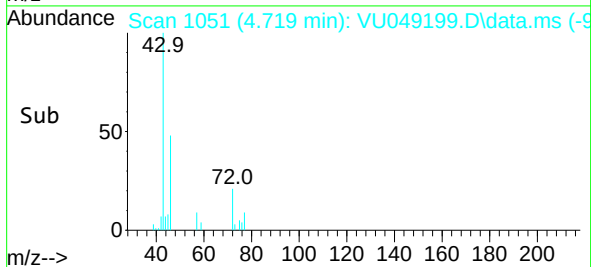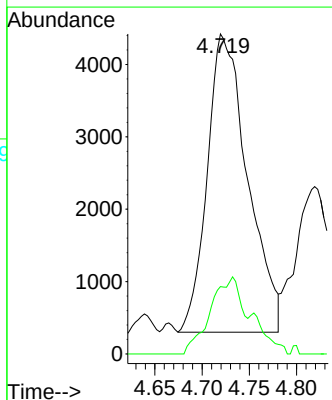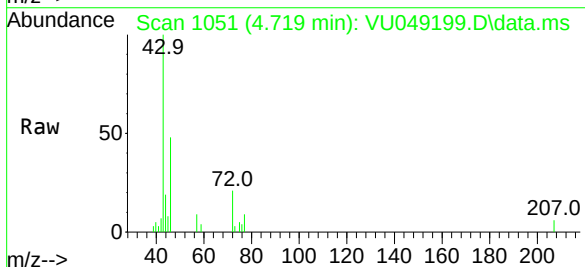

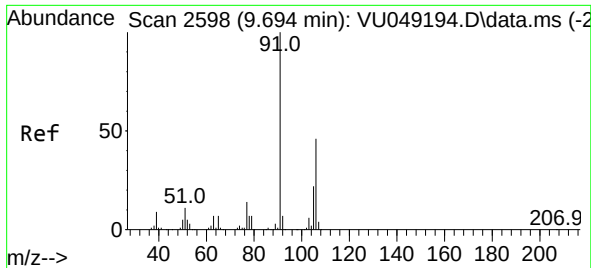

#53
 m,p-Xylene
 Concen: 0.102 ug/L
 RT: 9.693 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VU049199.D
 Acq: 16 Jun 2022 11:56

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BF9

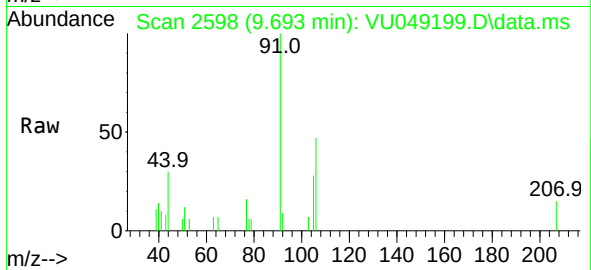

Tgt Ion:106 Resp: 1475
 Ion Ratio Lower Upper
 106 100
 91 213.8 148.5 275.7

