

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061622\
 Data File : VU049203.D
 Acq On : 16 Jun 2022 13:30
 Operator : SY/MD
 Sample : N3288-02DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGJ97DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049203.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	87	rBV	59403	69541	12.14%	1.538%
2	1.913	172	178	192	rVB	45814	60306	10.53%	1.334%
3	2.572	369	383	400	rBV3	107452	203287	35.50%	4.497%
4	3.048	519	531	547	rVB2	15055	28099	4.91%	0.622%
5	3.871	774	787	804	rBV2	6152	14352	2.51%	0.318%
6	4.636	1010	1025	1068	rBV	89290	285414	49.84%	6.314%
7	5.067	1139	1159	1177	rBV	84965	184854	32.28%	4.089%
8	5.726	1344	1364	1384	rBV3	172824	443220	77.40%	9.805%
9	6.250	1514	1527	1547	rBV	156819	300754	52.52%	6.653%
10	6.543	1605	1618	1637	rBV	224874	425219	74.26%	9.407%
11	6.694	1652	1665	1684	rBV	110601	217156	37.92%	4.804%
12	7.565	1921	1936	1955	rBV	59123	106583	18.61%	2.358%
13	7.900	2026	2040	2055	rBV	208679	365065	63.75%	8.076%
14	7.973	2056	2063	2073	rVB4	3056	6219	1.09%	0.138%
15	8.182	2117	2128	2142	rBV2	34878	59904	10.46%	1.325%
16	8.636	2255	2269	2302	rBV2	283592	572641	100.00%	12.668%
17	9.417	2499	2512	2533	rBV	210245	354554	61.92%	7.844%
18	10.758	2918	2929	2948	rVB	87088	140471	24.53%	3.108%
19	11.813	3245	3257	3274	rBV	217682	355379	62.06%	7.862%
20	12.195	3364	3376	3390	rBV	195018	327242	57.15%	7.239%




Sum of corrected areas: 4520260

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061622\
Data File : VU049203.D
Acq On : 16 Jun 2022 13:30
Operator : SY/MD
Sample : N3288-02DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGJ97DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

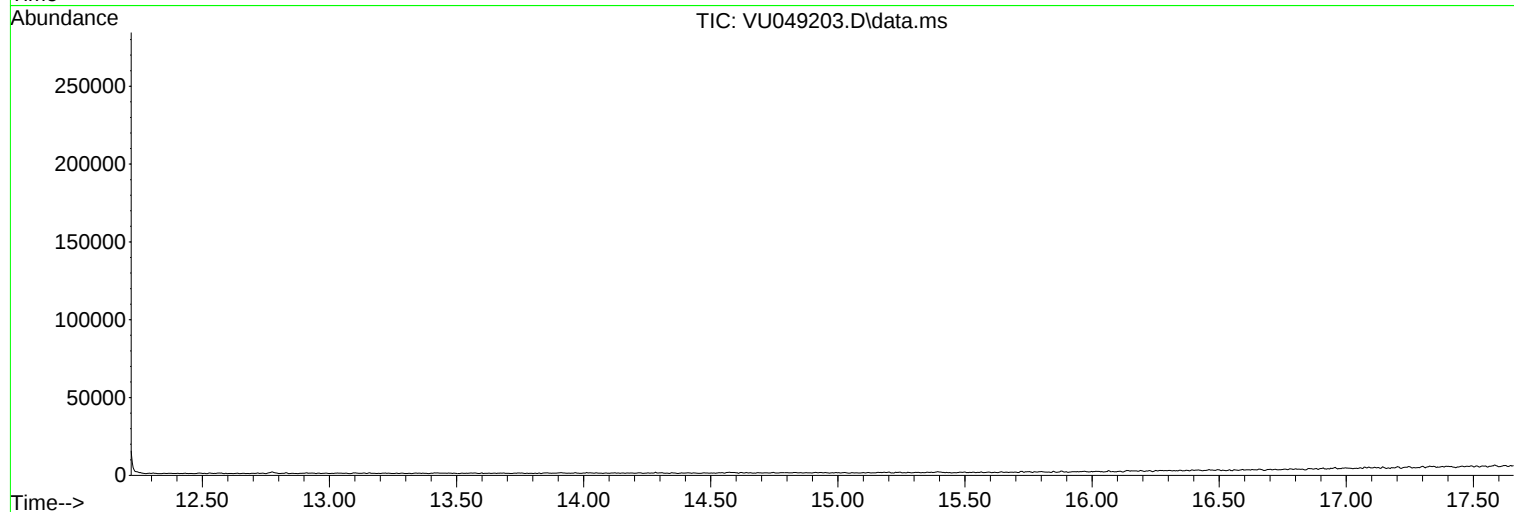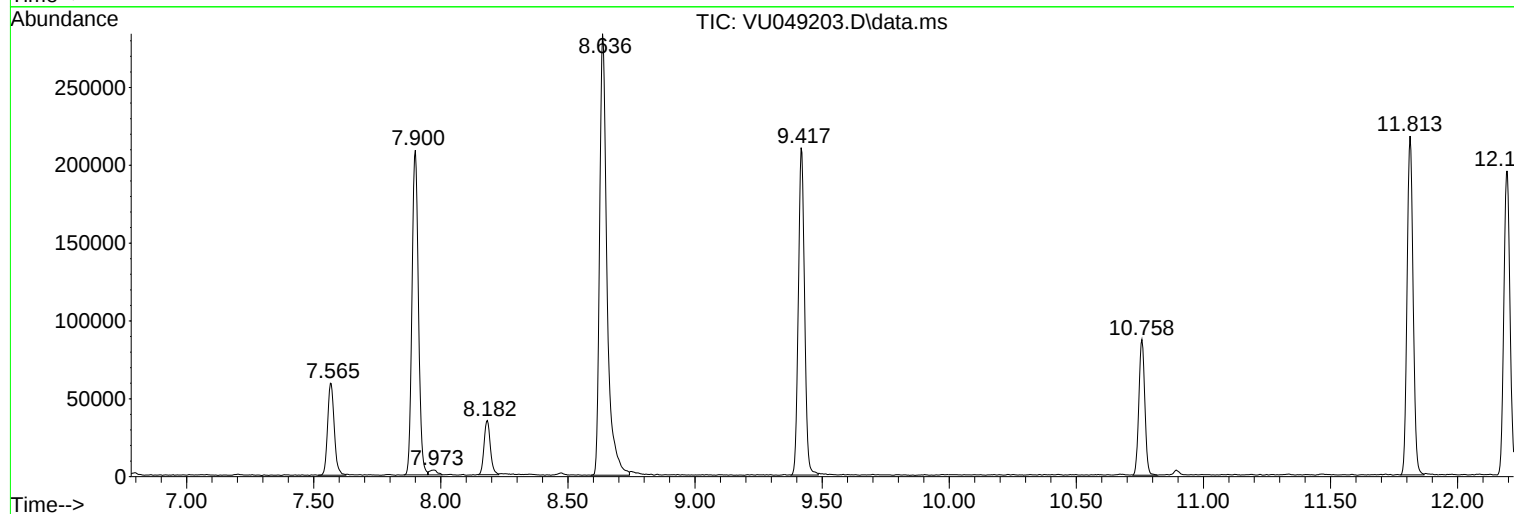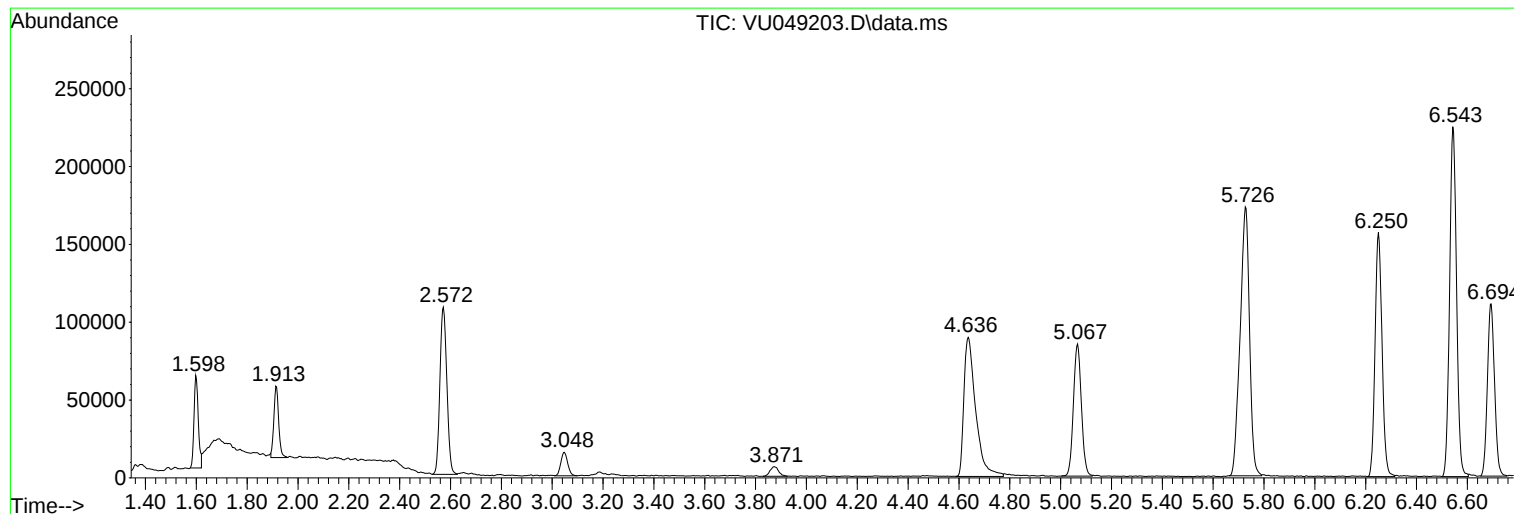

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061622\
Data File : VU049203.D
Acq On : 16 Jun 2022 13:30
Operator : SY/MD
Sample : N3288-02DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGJ97DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061622\
Data File : VU049203.D
Acq On : 16 Jun 2022 13:30
Operator : SY/MD
Sample : N3288-02DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGJ97DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc