

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061622\
 Data File : VU049207.D
 Acq On : 16 Jun 2022 15:05
 Operator : SY/MD
 Sample : N3277-06 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BA5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.517	40	55	65	rBV2	26718	86600	13.68%	1.883%
2	1.597	74	80	91	rBV	52258	62367	9.85%	1.356%
3	1.912	171	178	190	rVB	43760	57528	9.09%	1.251%
4	2.568	370	382	396	rBV	80398	129838	20.50%	2.823%
5	3.047	517	531	547	rVB2	27069	52334	8.26%	1.138%
6	3.186	558	574	587	rBV2	8563	20142	3.18%	0.438%
7	4.639	1008	1026	1067	rBV2	99603	333819	52.72%	7.258%
8	5.067	1141	1159	1185	rVB	81930	183383	28.96%	3.987%
9	5.726	1341	1364	1390	rBV2	168106	439730	69.44%	9.561%
10	6.250	1513	1527	1547	rBV	160100	306555	48.41%	6.665%
11	6.542	1604	1618	1638	rBV	181731	344058	54.34%	7.481%
12	6.694	1652	1665	1687	rVB	108931	212342	33.53%	4.617%
13	7.568	1922	1937	1954	rBV2	58826	105169	16.61%	2.287%
14	7.899	2026	2040	2056	rBV	201107	354485	55.98%	7.707%
15	7.970	2056	2062	2072	rVB2	4010	6587	1.04%	0.143%
16	8.182	2117	2128	2143	rBV	35291	61329	9.69%	1.333%
17	8.636	2257	2269	2309	rBV2	309565	633214	100.00%	13.768%
18	9.417	2500	2512	2539	rBV	219919	367554	58.05%	7.991%
19	10.758	2916	2929	2942	rBV	90932	147587	23.31%	3.209%
20	11.812	3244	3257	3275	rBV	231023	366720	57.91%	7.973%
21	12.195	3364	3376	3396	rBV	198999	327995	51.80%	7.131%




Sum of corrected areas: 4599336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061622\
Data File : VU049207.D
Acq On : 16 Jun 2022 15:05
Operator : SY/MD
Sample : N3277-06 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

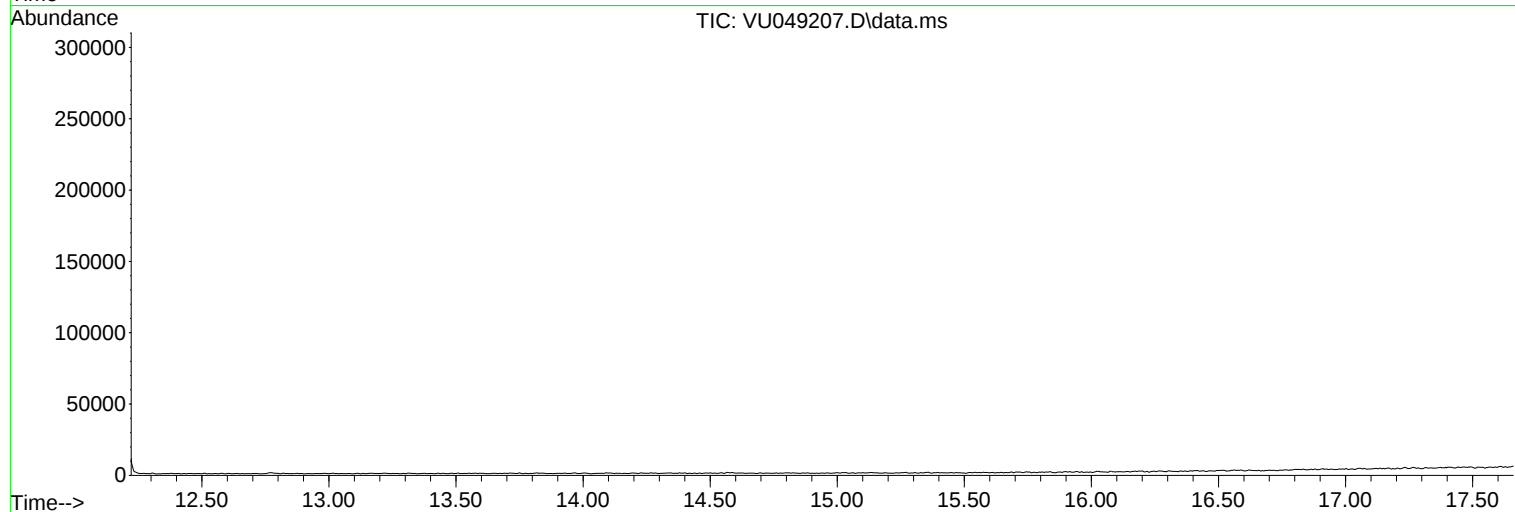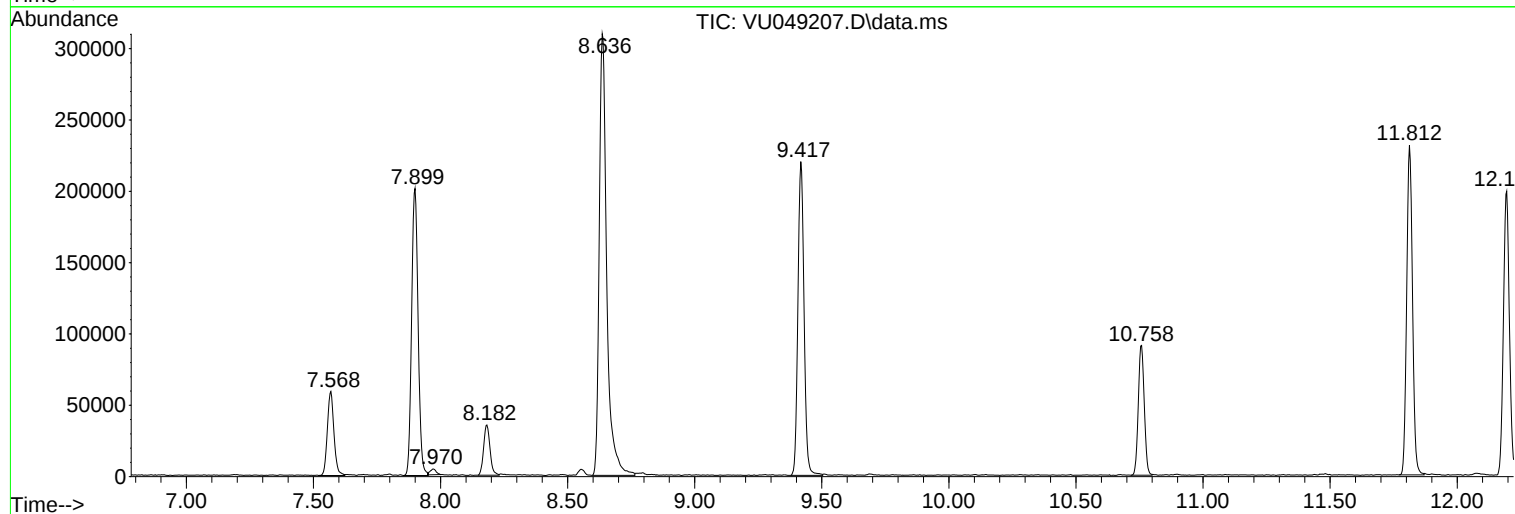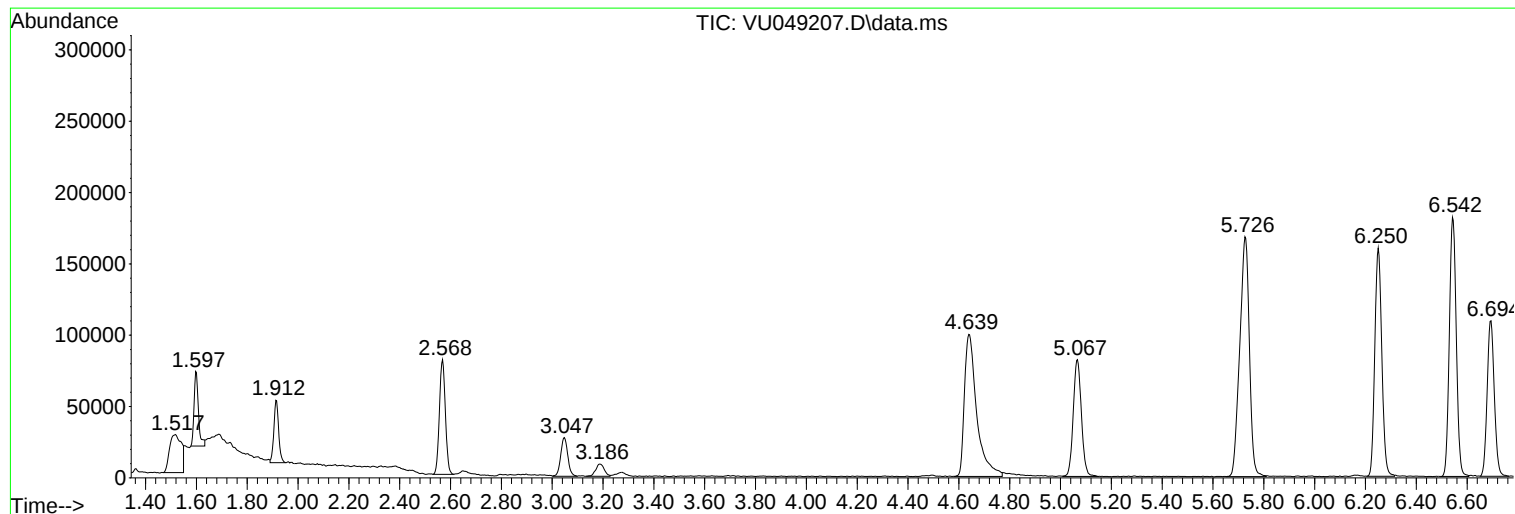

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061622\
Data File : VU049207.D
Acq On : 16 Jun 2022 15:05
Operator : SY/MD
Sample : N3277-06 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.517	1.4	ug/L	86600	1	6.250	306555	5.0