


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061622\
 Data File : VU049193.D
 Acq On : 16 Jun 2022 08:47
 Operator : SY/MD
 Sample : BFB084
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB084

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jun 18 05:20:12 2022

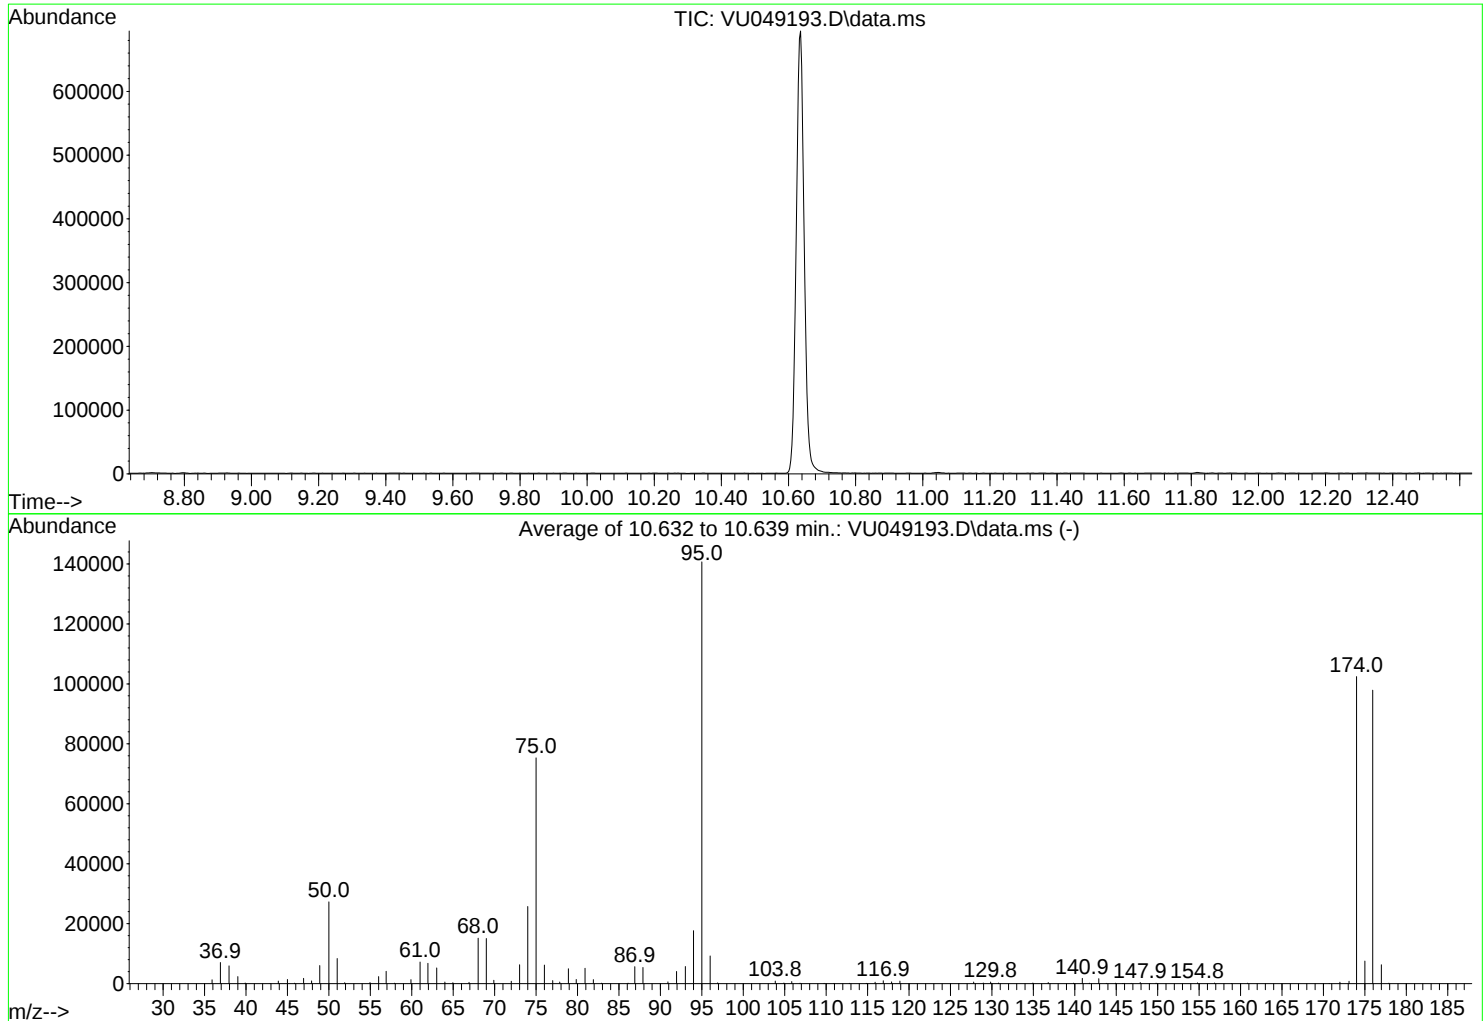

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	27259	PASS
75	95	30	80	53.5	75304	PASS
95	95	100	100	100.0	140715	PASS
96	95	5	9	6.6	9218	PASS
173	174	0.00	2	0.8	776	PASS
174	95	50	120	72.8	102453	PASS
175	174	5	9	7.3	7524	PASS
176	174	95	101	95.6	97896	PASS
177	176	5	9	6.4	6293	PASS

m/z	Abundance
40.00	187.0
43.90	567.0
207.00	305.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084

m/z	Abundance
35.90	1429.0
36.90	7531.0
38.00	6209.0
39.00	2398.0
39.90	350.0
43.90	1505.0
45.00	1467.0
45.90	153.0
46.90	1921.0
47.90	942.0
48.90	6123.0
50.00	28440.0
51.00	8712.0
51.90	314.0
54.90	338.0
56.00	2395.0
56.90	4214.0
57.90	234.0
59.90	1457.0
61.00	7386.0
62.00	6939.0
63.00	5434.0
64.00	482.0
64.90	329.0
66.90	404.0
68.00	15698.0
69.00	15449.0
69.90	1172.0
72.00	844.0
73.00	6607.0
74.00	26320.0
75.00	77808.0
76.00	6462.0
77.00	1105.0
77.80	521.0
78.90	5148.0
79.90	1414.0
80.90	5281.0
81.90	1256.0
82.90	124.0
86.10	219.0
86.90	5835.0
87.90	5487.0
90.90	608.0
91.90	4139.0
93.00	5798.0
94.00	17984.0
95.00	142976.0
96.00	9786.0
96.90	257.0
103.80	857.0
104.90	219.0
105.80	743.0
106.90	190.0
109.80	120.0
110.90	141.0
112.80	132.0
114.80	118.0
115.90	496.0
116.90	1012.0
117.90	531.0
118.90	895.0
127.80	531.0
128.90	253.0
129.80	565.0
130.80	196.0
134.90	200.0
136.80	335.0
139.80	150.0
140.90	1672.0
141.80	188.0
142.90	1699.0
143.80	135.0
144.90	192.0
145.80	152.0
146.80	118.0
147.90	419.0
149.80	146.0
154.80	332.0
156.80	225.0
160.90	139.0
172.00	524.0
174.00	101312.0
175.00	7573.0
176.00	98024.0
177.00	6328.0
177.90	177.0
206.90	273.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084

m/z	Abundance
35.90	1320.0
36.90	7232.0
37.90	6088.0
39.00	2454.0
39.90	404.0
43.90	1487.0
45.00	1415.0
45.80	153.0
46.90	1838.0
47.90	981.0
48.90	6246.0
50.00	28144.0
51.00	8702.0
51.90	348.0
55.00	384.0
56.00	2464.0
56.90	4330.0
57.90	176.0
59.90	1391.0
61.00	7448.0
62.00	6931.0
63.00	5375.0
64.00	538.0
64.90	314.0
66.90	435.0
68.00	15746.0
69.00	15622.0
69.90	1142.0
72.00	820.0
73.00	6451.0
74.00	26640.0
75.00	77904.0
76.00	6350.0
77.00	1106.0
77.90	563.0
78.90	5112.0
79.90	1428.0
80.90	5327.0
81.90	1378.0
82.90	153.0
86.10	221.0
86.90	5805.0
87.90	5560.0
90.90	596.0
91.90	4142.0
93.00	5846.0
94.00	18240.0
95.00	145088.0
96.00	9452.0
96.90	256.0
103.90	863.0
104.90	200.0
105.80	721.0
106.80	191.0
109.80	117.0
110.90	138.0
112.80	134.0
114.80	122.0
115.90	487.0
116.90	987.0
117.90	599.0
118.90	952.0
127.80	540.0
129.00	208.0
129.80	587.0
130.80	215.0
135.00	234.0
136.80	361.0
139.80	146.0
140.90	1855.0
141.80	144.0
142.90	1670.0
143.80	152.0
144.90	184.0
146.00	154.0
146.80	131.0
147.90	397.0
149.00	117.0
149.80	168.0
154.80	287.0
156.80	245.0
158.90	116.0
160.80	151.0
170.70	120.0
172.00	497.0
173.10	1270.0
174.00	105992.0
175.00	7703.0
175.90	101024.0
177.00	6446.0
177.90	201.0
207.00	293.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084

m/z	Abundance
35.90	1155.0
36.90	6411.0
37.90	5509.0
39.00	2259.0
39.90	387.0
42.90	112.0
43.90	1366.0
45.00	1309.0
45.80	149.0
47.00	1594.0
47.90	871.0
48.90	5691.0
50.00	25192.0
51.00	7720.0
51.90	321.0
55.00	383.0
56.00	2224.0
56.90	3879.0
57.90	111.0
59.90	1231.0
61.00	6836.0
61.90	6513.0
63.00	4906.0
64.00	538.0
65.00	285.0
66.90	433.0
68.00	14053.0
69.00	14109.0
69.90	1061.0
72.00	712.0
73.00	5801.0
74.00	24256.0
75.00	70200.0
76.00	5757.0
77.00	920.0
77.80	538.0
78.90	4631.0
79.80	1292.0
80.90	4818.0
81.90	1313.0
82.90	164.0
86.90	5333.0
87.90	5086.0
90.90	545.0
92.00	3835.0
93.00	5492.0
94.00	16784.0
95.00	134080.0
96.00	8417.0
96.90	252.0
103.90	779.0
104.90	185.0
105.90	657.0
106.80	180.0
109.70	102.0
111.00	111.0
112.80	112.0
114.90	131.0
115.90	438.0
116.90	910.0
117.90	623.0
118.90	811.0
126.00	105.0
127.80	488.0
129.00	187.0
129.90	542.0
130.80	205.0
135.00	256.0
136.80	362.0
139.90	129.0
140.90	1737.0
141.70	132.0
142.90	1625.0
143.80	115.0
144.90	155.0
145.90	151.0
146.80	121.0
147.90	341.0
149.10	115.0
149.80	134.0
154.80	234.0
156.90	243.0
158.90	130.0
160.80	158.0
172.00	454.0
173.10	1058.0
174.00	100056.0
175.00	7295.0
175.90	94640.0
177.00	6106.0
177.90	174.0
207.00	330.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084