

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
 Data File : VU049289.D
 Acq On : 18 Jun 2022 18:21
 Operator : SY/MD
 Sample : N3313-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Jun 20 00:14:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jun 20 00:11:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	254385	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	240616	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	111640	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	75299	48.049	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	96.100%
7) Chloroethane-d5	1.912	69	59696	51.880	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.760%
11) 1,1-Dichloroethene-d2	2.565	63	104530	35.349	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.700%
21) 2-Butanone-d5	4.626	46	199743	116.252	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	116.250%
24) Chloroform-d	5.063	84	161461	48.297	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.600%
26) 1,2-Dichloroethane-d4	5.700	65	110720	51.120	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.240%
32) Benzene-d6	5.726	84	311516	52.211	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.420%
36) 1,2-Dichloropropane-d6	6.690	67	116213	57.939	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	115.880%
41) Toluene-d8	7.899	98	278083	52.848	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.700%
43) trans-1,3-Dichloroprop...	8.179	79	49504	52.462	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	104.920%
47) 2-Hexanone-d5	8.632	63	129524	123.383	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	123.380%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	174583	52.113	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	104.220%
66) 1,2-Dichlorobenzene-d4	12.192	152	111628	57.467	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	114.940%
Target Compounds						
					Qvalue	
13) Acetone	2.639	43	6453	4.773	ug/L	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
Data File : VU049289.D
Acq On : 18 Jun 2022 18:21
Operator : SY/MD
Sample : N3313-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: Jun 20 00:14:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Jun 20 00:11:46 2022
Response via : Initial Calibration

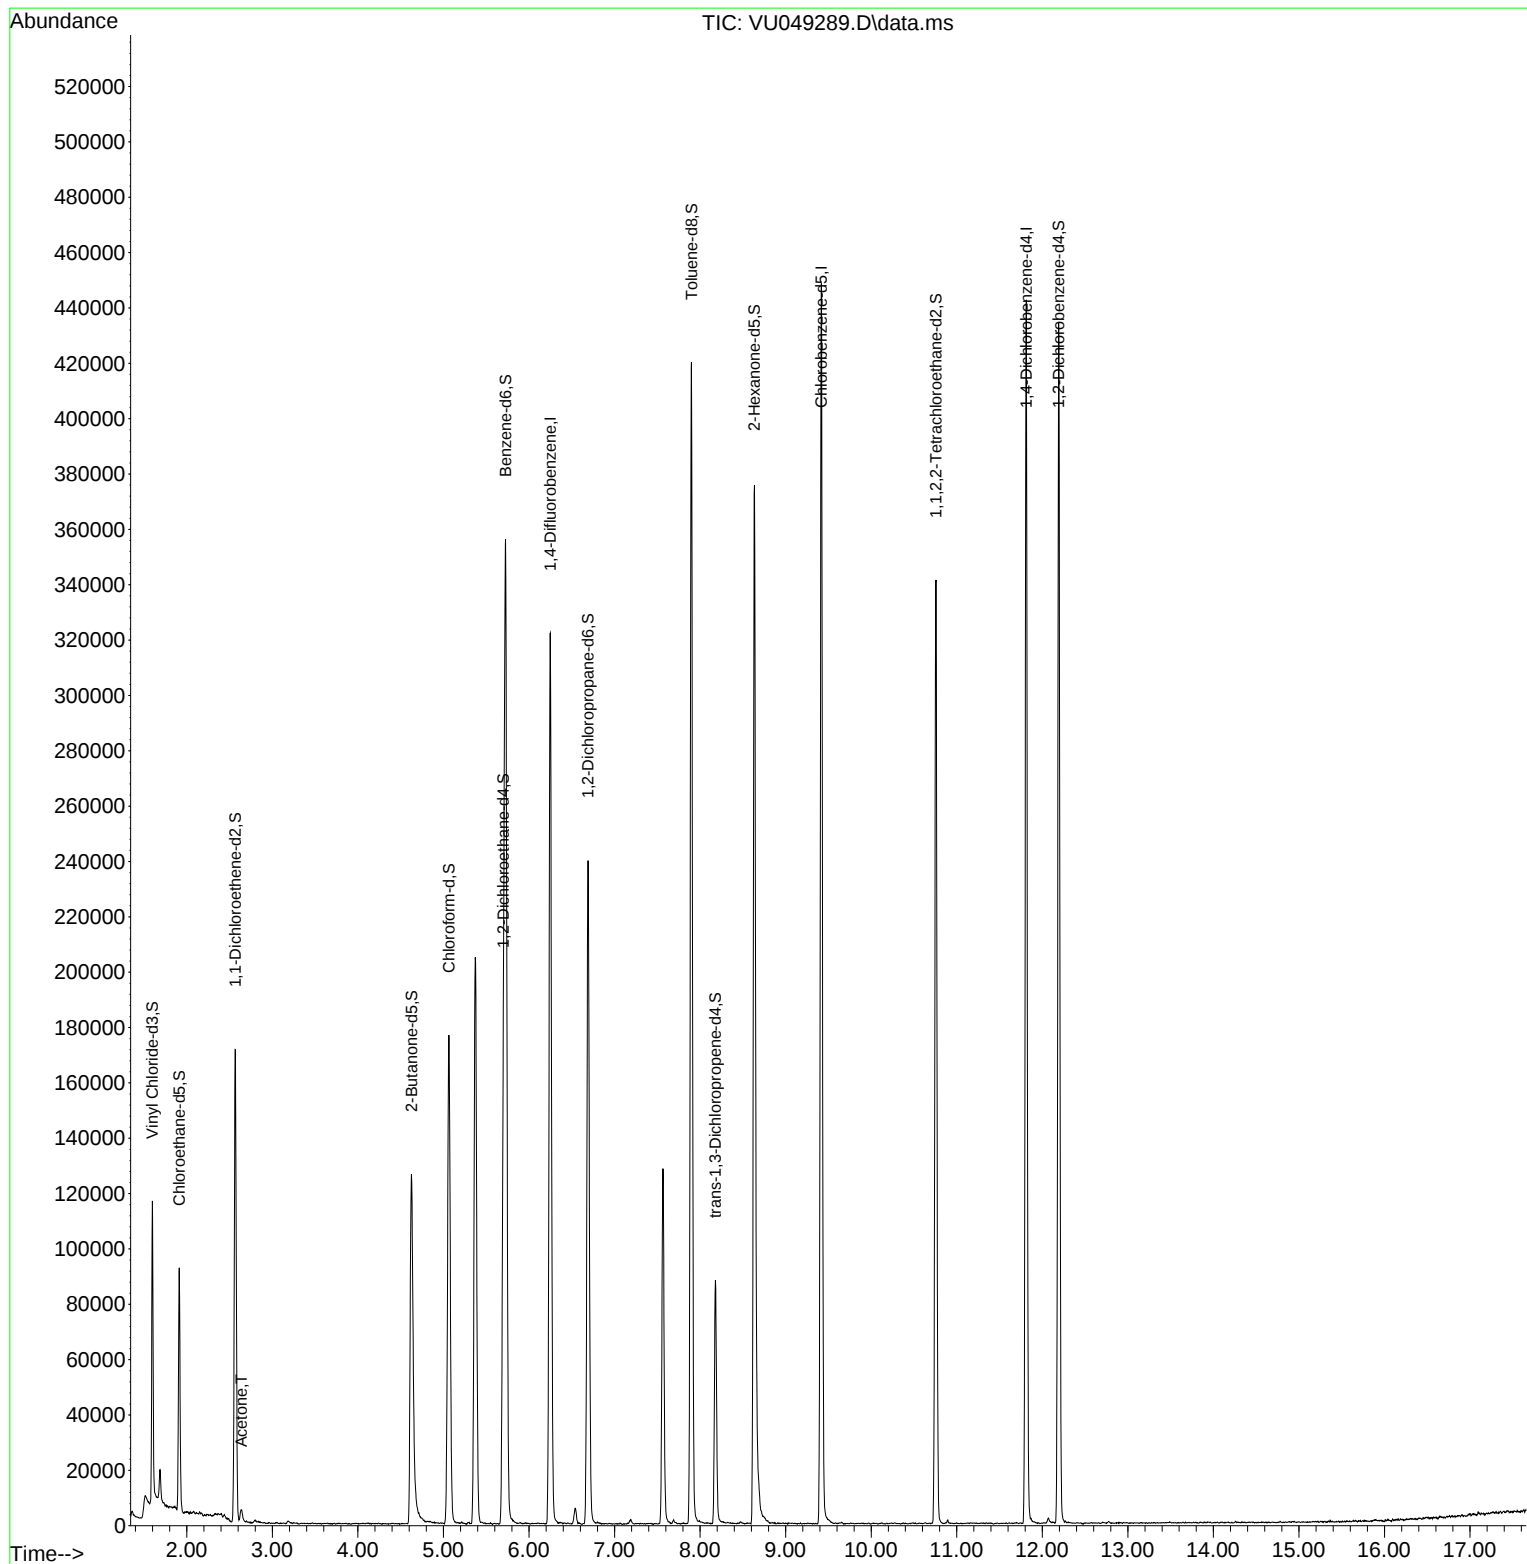


Abundance Scan 400 (2.626 min): VU049279.D\data.ms (-38

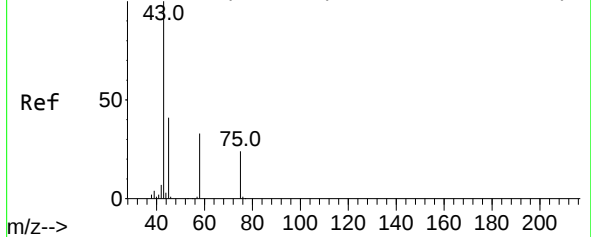

Abundance Scan 404 (2.639 min): VU049289.D\data.ms

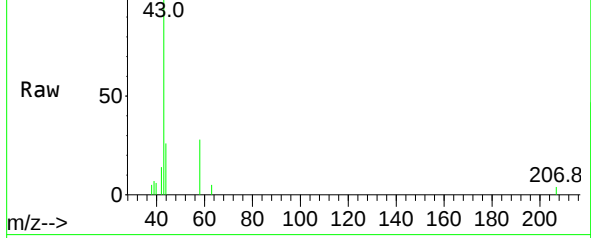

Abundance Scan 404 (2.639 min): VU049289.D\data.ms (-30

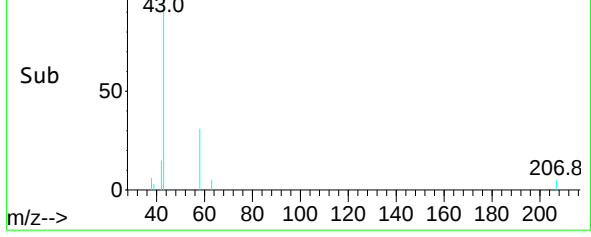

#13

Acetone

Concen: 4.773 ug/L

RT: 2.639 min Scan# 40

Delta R.T. 0.013 min

Lab File: VU049289.D

Acq: 18 Jun 2022 18:21

Instrument :

MSVOA_U

ClientSampleId :

VHBLK001

Tgt Ion: 43 Resp: 6453

Ion Ratio Lower Upper

43 100

58 16.4 0.0 66.4

