

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
 Data File : VU049288.D
 Acq On : 18 Jun 2022 17:58
 Operator : SY/MD
 Sample : N3313-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YB7L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049288.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.478	35	43	55	rBV	14079	32325	2.05%	0.322%
2	1.597	74	80	94	rBV	104766	115348	7.32%	1.150%
3	1.912	170	178	190	rVB	89212	108868	6.91%	1.086%
4	2.568	370	382	397	rBV2	170542	287674	18.26%	2.869%
5	2.742	434	436	437	rBV	544	233	0.01%	0.002%
6	2.867	472	475	479	rBV2	278	262	0.02%	0.003%
7	3.051	526	532	539	rVB4	660	1145	0.07%	0.011%
8	3.089	539	544	545	rBV	479	350	0.02%	0.003%
9	3.183	560	573	583	rBV3	1740	3850	0.24%	0.038%
10	3.369	629	631	634	rVB3	470	256	0.02%	0.003%
11	3.462	657	660	665	rVB3	465	312	0.02%	0.003%
12	3.732	739	744	750	rVB2	276	300	0.02%	0.003%
13	3.874	782	788	792	rVB3	600	530	0.03%	0.005%
14	4.131	860	868	871	rBV3	374	524	0.03%	0.005%
15	4.182	881	884	888	rVB3	285	222	0.01%	0.002%
16	4.340	929	933	937	rBV2	310	298	0.02%	0.003%
17	4.620	1007	1020	1048	rBV	124864	305117	19.36%	3.043%
18	4.777	1067	1069	1074	rVB3	477	292	0.02%	0.003%
19	4.967	1122	1128	1132	rVB3	254	312	0.02%	0.003%
20	5.063	1142	1158	1179	rBV2	170815	381230	24.19%	3.802%
21	5.173	1189	1192	1199	rVB5	734	841	0.05%	0.008%
22	5.211	1199	1204	1209	rBV5	484	664	0.04%	0.007%
23	5.292	1225	1229	1232	rBV2	504	411	0.03%	0.004%
24	5.372	1239	1254	1277	rBV	205819	429204	27.24%	4.280%
25	5.530	1299	1303	1306	rBV3	317	296	0.02%	0.003%
26	5.726	1342	1364	1386	rBV2	342861	937598	59.50%	9.350%
27	6.051	1462	1465	1467	rBV	402	270	0.02%	0.003%
28	6.112	1482	1484	1491	rBV3	276	247	0.02%	0.002%
29	6.247	1508	1526	1553	rBV	327906	622725	39.52%	6.210%
30	6.543	1603	1618	1650	rVV	837059	1575856	100.00%	15.715%
31	6.690	1650	1664	1689	rVB	233680	459416	29.15%	4.581%
32	6.806	1695	1700	1702	rBV4	652	586	0.04%	0.006%
33	6.973	1749	1752	1755	rBV	379	275	0.02%	0.003%
34	7.006	1758	1762	1766	rVV	281	234	0.01%	0.002%
35	7.070	1777	1782	1786	rBV2	447	517	0.03%	0.005%
36	7.115	1793	1796	1802	rVB2	384	296	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
 Data File : VU049288.D
 Acq On : 18 Jun 2022 17:58
 Operator : SY/MD
 Sample : N3313-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YB7L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	7.186	1809	1818	1828	rVV4	1629	2728	0.17%	0.027%
38	7.337	1862	1865	1873	rVB3	211	245	0.02%	0.002%
39	7.565	1923	1936	1960	rBV	127369	224096	14.22%	2.235%
40	7.668	1965	1968	1969	rBV3	527	311	0.02%	0.003%
41	7.764	1995	1998	2002	rVB3	288	231	0.01%	0.002%
42	7.793	2002	2007	2011	rBV4	517	629	0.04%	0.006%
43	7.896	2026	2039	2063	rBV	407644	720816	45.74%	7.188%
44	8.089	2096	2099	2103	rVB	492	411	0.03%	0.004%
45	8.115	2103	2107	2112	rBV2	429	304	0.02%	0.003%
46	8.179	2112	2127	2145	rBV	89832	152408	9.67%	1.520%
47	8.375	2187	2188	2192	rVB	453	224	0.01%	0.002%
48	8.420	2199	2202	2207	rVB2	345	249	0.02%	0.002%
49	8.468	2210	2217	2221	rBV3	817	959	0.06%	0.010%
50	8.552	2231	2243	2256	rBV	134040	224158	14.22%	2.235%
51	8.632	2256	2268	2293	rBV	350036	651180	41.32%	6.494%
52	8.787	2308	2316	2329	rVB3	10439	17848	1.13%	0.178%
53	8.944	2363	2365	2370	rVB2	337	235	0.01%	0.002%
54	8.983	2373	2377	2381	rBV2	323	284	0.02%	0.003%
55	9.202	2439	2445	2449	rBV2	203	257	0.02%	0.003%
56	9.224	2449	2452	2455	rBV2	269	225	0.01%	0.002%
57	9.301	2471	2476	2478	rBV2	338	288	0.02%	0.003%
58	9.417	2499	2512	2534	rBV	462683	766640	48.65%	7.645%
59	9.568	2556	2559	2562	rVB2	429	228	0.01%	0.002%
60	9.626	2568	2577	2578	rBV2	297	415	0.03%	0.004%
61	9.658	2585	2587	2589	rBV	424	264	0.02%	0.003%
62	9.739	2607	2612	2617	rBV3	317	327	0.02%	0.003%
63	10.073	2711	2716	2720	rBV2	417	554	0.04%	0.006%
64	10.169	2743	2746	2753	rBV2	185	238	0.02%	0.002%
65	10.279	2777	2780	2787	rBV2	319	229	0.01%	0.002%
66	10.346	2795	2801	2807	rVB3	786	762	0.05%	0.008%
67	10.407	2816	2820	2826	rBV2	330	319	0.02%	0.003%
68	10.655	2893	2897	2900	rBV2	346	261	0.02%	0.003%
69	10.755	2916	2928	2948	rBV	335877	546223	34.66%	5.447%
70	10.890	2967	2970	2974	rBV3	657	426	0.03%	0.004%
71	11.034	3010	3015	3018	rBV3	319	395	0.03%	0.004%
72	11.208	3065	3069	3072	rBV3	402	395	0.03%	0.004%
73	11.230	3073	3076	3079	rVV2	298	230	0.01%	0.002%
74	11.298	3090	3097	3099	rBV2	394	470	0.03%	0.005%
75	11.423	3133	3136	3142	rVB2	277	247	0.02%	0.002%
76	11.562	3176	3179	3182	rVB	314	227	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
 Data File : VU049288.D
 Acq On : 18 Jun 2022 17:58
 Operator : SY/MD
 Sample : N3313-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YB7L6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.581	3182	3185	3188	rBV	335	299	0.02%	0.003%
78	11.665	3207	3211	3212	rBV2	415	282	0.02%	0.003%
79	11.697	3214	3221	3229	rVB6	4010	6183	0.39%	0.062%
80	11.812	3244	3257	3273	rBV	444756	721658	45.79%	7.197%
81	12.134	3352	3357	3359	rVV2	349	300	0.02%	0.003%
82	12.192	3362	3375	3399	rVV	432832	698641	44.33%	6.967%
83	12.430	3446	3449	3456	rVB2	268	272	0.02%	0.003%
84	12.484	3463	3466	3472	rVB	363	269	0.02%	0.003%
85	12.513	3472	3475	3480	rVB3	435	357	0.02%	0.004%
86	12.780	3550	3558	3565	rVB2	443	714	0.05%	0.007%
87	12.822	3565	3571	3573	rBV3	322	308	0.02%	0.003%
88	12.893	3587	3593	3605	rVV5	4488	7301	0.46%	0.073%
89	13.176	3678	3681	3687	rVB2	459	349	0.02%	0.003%
90	13.455	3763	3768	3774	rBV2	438	505	0.03%	0.005%
91	13.600	3807	3813	3817	rBV2	398	447	0.03%	0.004%
92	13.844	3887	3889	3894	rVB3	379	223	0.01%	0.002%
93	14.237	4008	4011	4015	rBV2	375	299	0.02%	0.003%
94	14.455	4076	4079	4082	rBV	411	292	0.02%	0.003%
95	14.941	4227	4230	4233	rBV2	351	309	0.02%	0.003%
96	15.028	4254	4257	4261	rVB2	507	340	0.02%	0.003%
97	15.243	4318	4324	4330	rBV4	467	725	0.05%	0.007%
98	15.687	4458	4462	4465	rBV2	548	487	0.03%	0.005%
99	15.979	4550	4553	4555	rBV3	498	295	0.02%	0.003%
100	16.169	4607	4612	4617	rBV7	766	1102	0.07%	0.011%




Sum of corrected areas: 10027777

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
Data File : VU049288.D
Acq On : 18 Jun 2022 17:58
Operator : SY/MD
Sample : N3313-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YB7L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

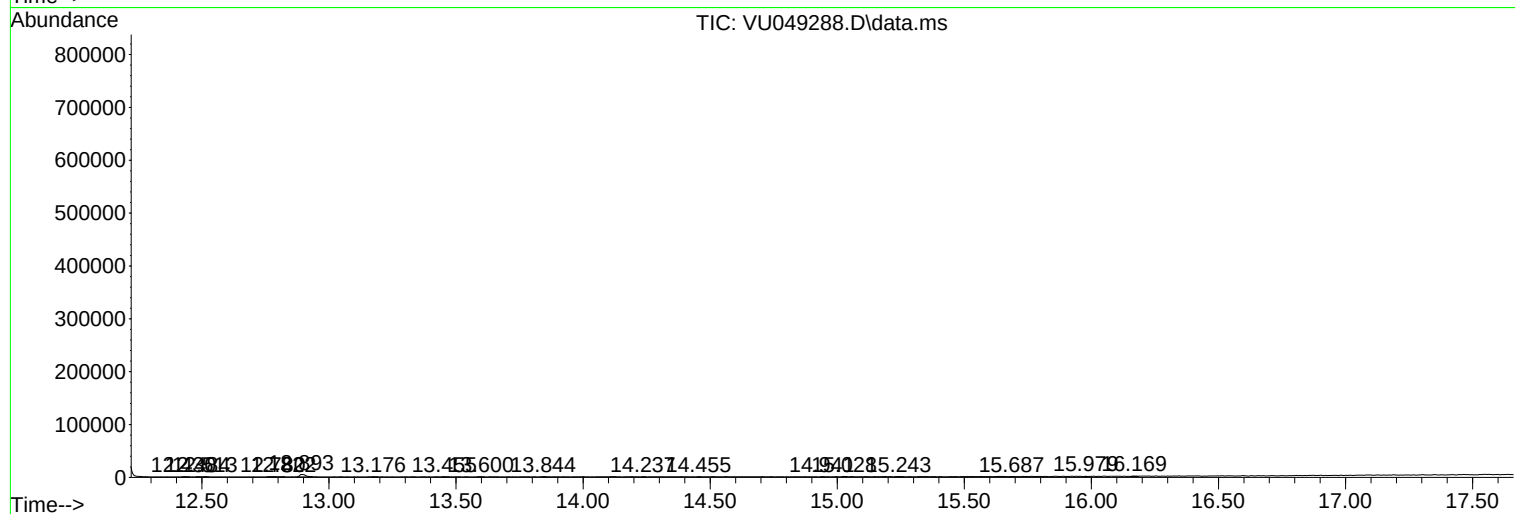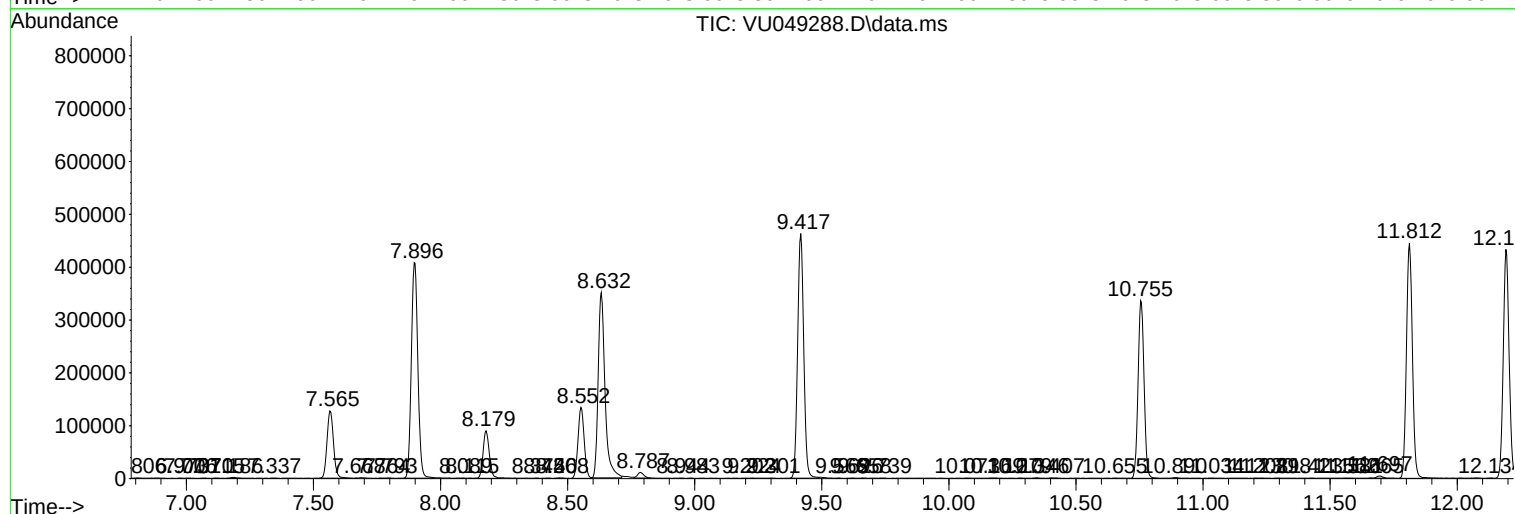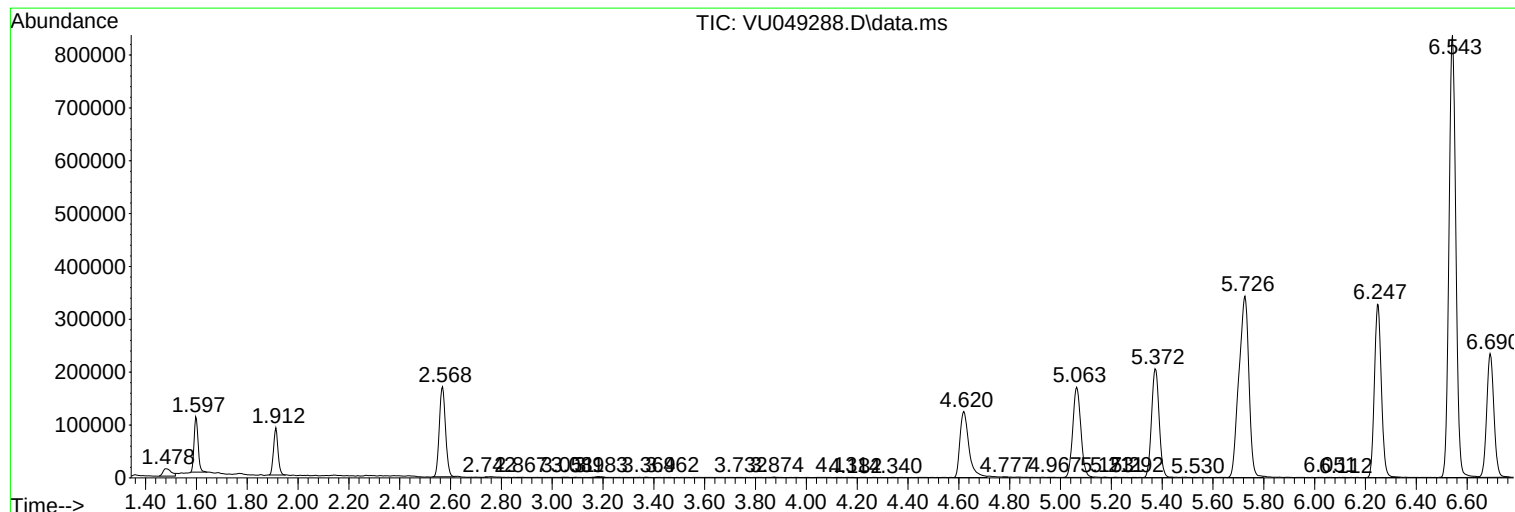

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
Data File : VU049288.D
Acq On : 18 Jun 2022 17:58
Operator : SY/MD
Sample : N3313-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YB7L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.478	2.6	ug/L	32325	1	6.250	622725	50.0