

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
 Data File : VU049289.D
 Acq On : 18 Jun 2022 18:21
 Operator : SY/MD
 Sample : N3313-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049289.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	108565	122806	12.82%	1.481%
2	1.912	170	178	192	rVB	88499	114113	11.91%	1.376%
3	2.565	369	381	395	rBV	170553	277283	28.94%	3.344%
4	2.639	397	404	419	rVB2	4454	8841	0.92%	0.107%
5	2.739	433	435	439	rVB	499	268	0.03%	0.003%
6	2.855	469	471	475	rVB2	374	215	0.02%	0.003%
7	2.903	484	486	491	rVB	365	324	0.03%	0.004%
8	2.964	500	505	510	rVB2	420	458	0.05%	0.006%
9	3.051	530	532	538	rVB4	440	371	0.04%	0.004%
10	3.128	550	556	561	rBV3	233	347	0.04%	0.004%
11	3.186	568	574	582	rBV4	790	1426	0.15%	0.017%
12	3.250	591	594	597	rBV2	433	367	0.04%	0.004%
13	3.289	602	606	609	rVB2	362	311	0.03%	0.004%
14	3.343	614	623	626	rBV3	310	493	0.05%	0.006%
15	3.758	745	752	754	rBV	292	275	0.03%	0.003%
16	3.941	804	809	814	rBV3	274	371	0.04%	0.004%
17	4.240	899	902	908	rBV3	256	242	0.03%	0.003%
18	4.469	970	973	978	rVB2	293	293	0.03%	0.004%
19	4.626	1008	1022	1047	rBV	126362	316614	33.04%	3.819%
20	4.893	1103	1105	1107	rVB	508	232	0.02%	0.003%
21	5.063	1142	1158	1180	rBV	176556	387642	40.46%	4.675%
22	5.215	1201	1205	1208	rBV2	550	431	0.04%	0.005%
23	5.282	1223	1226	1227	rBV2	536	262	0.03%	0.003%
24	5.372	1239	1254	1273	rVV	204587	425278	44.38%	5.129%
25	5.481	1285	1288	1292	rVB2	357	336	0.04%	0.004%
26	5.549	1306	1309	1314	rVB2	335	260	0.03%	0.003%
27	5.597	1317	1324	1328	rBV3	388	601	0.06%	0.007%
28	5.633	1332	1335	1340	rVB2	255	243	0.03%	0.003%
29	5.726	1342	1364	1386	rBV2	355774	958192	100.00%	11.557%
30	5.954	1432	1435	1440	rBV3	341	275	0.03%	0.003%
31	6.170	1499	1502	1508	rVB3	295	298	0.03%	0.004%
32	6.250	1512	1527	1555	rVV	321892	615555	64.24%	7.424%
33	6.539	1604	1617	1627	rBV10	5681	11108	1.16%	0.134%
34	6.636	1642	1647	1649	rBV	330	286	0.03%	0.003%
35	6.690	1649	1664	1690	rVV	239681	467075	48.75%	5.633%
36	6.800	1696	1698	1702	rVB4	409	237	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
 Data File : VU049289.D
 Acq On : 18 Jun 2022 18:21
 Operator : SY/MD
 Sample : N3313-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.838	1708	1710	1714	rVB2	423	234	0.02%	0.003%
38	6.861	1714	1717	1722	rBV2	273	279	0.03%	0.003%
39	6.938	1736	1741	1744	rBV3	277	263	0.03%	0.003%
40	6.986	1752	1756	1761	rBV3	156	212	0.02%	0.003%
41	7.015	1761	1765	1769	rVB3	311	284	0.03%	0.003%
42	7.041	1769	1773	1776	rBV3	268	213	0.02%	0.003%
43	7.067	1777	1781	1789	rVB2	556	631	0.07%	0.008%
44	7.112	1789	1795	1798	rBV2	319	328	0.03%	0.004%
45	7.134	1798	1802	1804	rBV2	262	219	0.02%	0.003%
46	7.153	1804	1808	1811	rBV2	373	299	0.03%	0.004%
47	7.179	1811	1816	1817	rVV2	1122	904	0.09%	0.011%
48	7.189	1817	1819	1831	rVB4	1618	1726	0.18%	0.021%
49	7.465	1901	1905	1908	rBV2	386	365	0.04%	0.004%
50	7.565	1923	1936	1956	rBV	128281	225256	23.51%	2.717%
51	7.690	1968	1975	1981	rBV3	1340	1744	0.18%	0.021%
52	7.793	2004	2007	2010	rVV2	271	235	0.02%	0.003%
53	7.899	2025	2040	2065	rBV	419548	738892	77.11%	8.912%
54	8.179	2115	2127	2149	rBV	87947	151050	15.76%	1.822%
55	8.468	2214	2217	2218	rBV	531	277	0.03%	0.003%
56	8.536	2234	2238	2241	rBV2	259	257	0.03%	0.003%
57	8.636	2256	2269	2300	rBV	375251	707808	73.87%	8.537%
58	8.874	2341	2343	2347	rVB3	508	321	0.03%	0.004%
59	8.909	2352	2354	2358	rVB2	386	224	0.02%	0.003%
60	9.015	2385	2387	2390	rVB2	393	247	0.03%	0.003%
61	9.031	2390	2392	2396	rBV2	484	450	0.05%	0.005%
62	9.144	2425	2427	2433	rBV3	250	284	0.03%	0.003%
63	9.173	2434	2436	2441	rVB2	427	240	0.03%	0.003%
64	9.211	2441	2448	2450	rBV2	203	243	0.03%	0.003%
65	9.263	2460	2464	2468	rVB3	258	216	0.02%	0.003%
66	9.324	2480	2483	2488	rBV2	288	268	0.03%	0.003%
67	9.417	2498	2512	2536	rBV	448209	752378	78.52%	9.074%
68	9.584	2560	2564	2570	rVB3	341	316	0.03%	0.004%
69	9.655	2583	2586	2593	rVB3	667	740	0.08%	0.009%
70	9.761	2615	2619	2622	rBV2	246	219	0.02%	0.003%
71	9.967	2679	2683	2690	rVB3	410	514	0.05%	0.006%
72	10.025	2695	2701	2704	rBV2	297	294	0.03%	0.004%
73	10.128	2728	2733	2737	rVB2	372	410	0.04%	0.005%
74	10.182	2744	2750	2754	rBV3	328	381	0.04%	0.005%
75	10.513	2851	2853	2858	rVB	325	216	0.02%	0.003%
76	10.758	2915	2929	2952	rVV	340911	559126	58.35%	6.744%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
 Data File : VU049289.D
 Acq On : 18 Jun 2022 18:21
 Operator : SY/MD
 Sample : N3313-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	10.893	2966	2971	2976	rVB3	1129	1098	0.11%	0.013%
78	10.996	3000	3003	3009	rVB3	283	219	0.02%	0.003%
79	11.163	3051	3055	3061	rBV2	290	357	0.04%	0.004%
80	11.314	3100	3102	3107	rVB2	323	215	0.02%	0.003%
81	11.343	3107	3111	3118	rBV2	300	434	0.05%	0.005%
82	11.449	3139	3144	3147	rBV3	256	257	0.03%	0.003%
83	11.472	3147	3151	3157	rVB2	285	322	0.03%	0.004%
84	11.700	3220	3222	3230	rVB2	375	349	0.04%	0.004%
85	11.812	3245	3257	3272	rBV	442119	706891	73.77%	8.526%
86	11.954	3298	3301	3306	rVB	326	282	0.03%	0.003%
87	12.073	3329	3338	3343	rBV2	1781	2635	0.27%	0.032%
88	12.121	3350	3353	3356	rBV2	381	286	0.03%	0.003%
89	12.192	3362	3375	3397	rBV	433536	710983	74.20%	8.575%
90	12.491	3464	3468	3471	rBV3	512	490	0.05%	0.006%
91	12.706	3532	3535	3539	rVV2	377	313	0.03%	0.004%
92	12.777	3550	3557	3561	rBV3	691	941	0.10%	0.011%
93	12.947	3607	3610	3614	rBV2	394	342	0.04%	0.004%
94	13.848	3885	3890	3892	rBV3	358	352	0.04%	0.004%
95	13.893	3901	3904	3908	rBV	438	316	0.03%	0.004%
96	13.931	3914	3916	3924	rBV3	374	432	0.05%	0.005%
97	14.079	3959	3962	3965	rBV2	352	270	0.03%	0.003%
98	14.922	4220	4224	4228	rBV3	392	436	0.05%	0.005%
99	15.365	4360	4362	4366	rVB2	569	249	0.03%	0.003%
100	16.008	4559	4562	4565	rBV2	691	464	0.05%	0.006%




Sum of corrected areas: 8291225

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
Data File : VU049289.D
Acq On : 18 Jun 2022 18:21
Operator : SY/MD
Sample : N3313-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

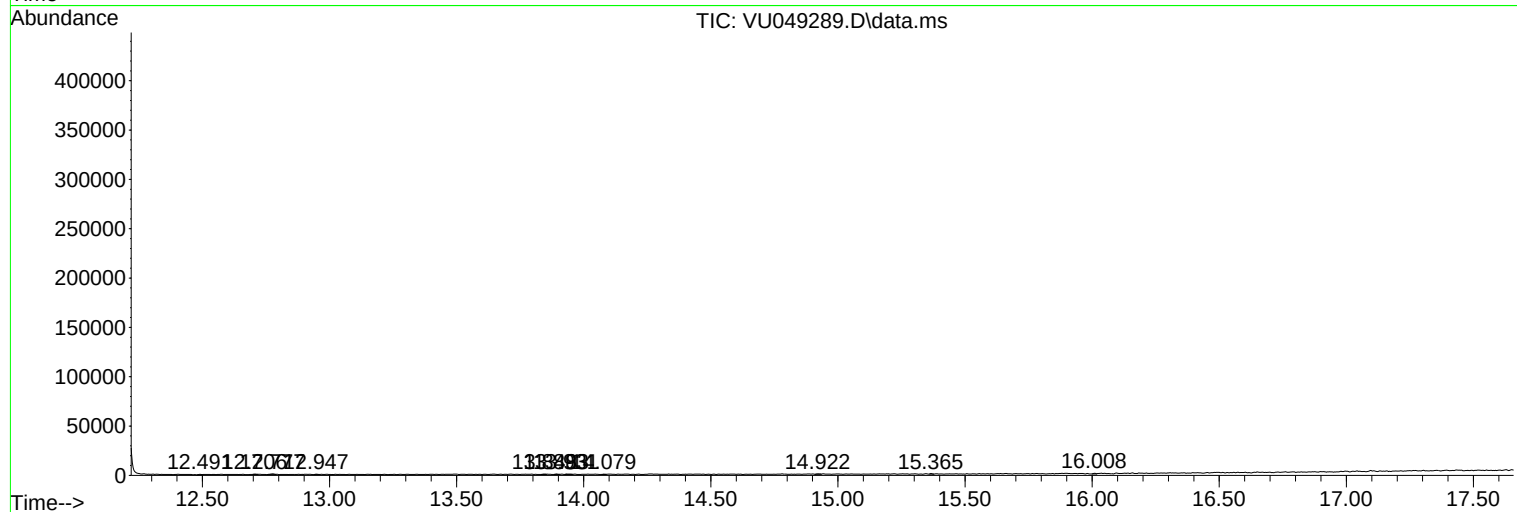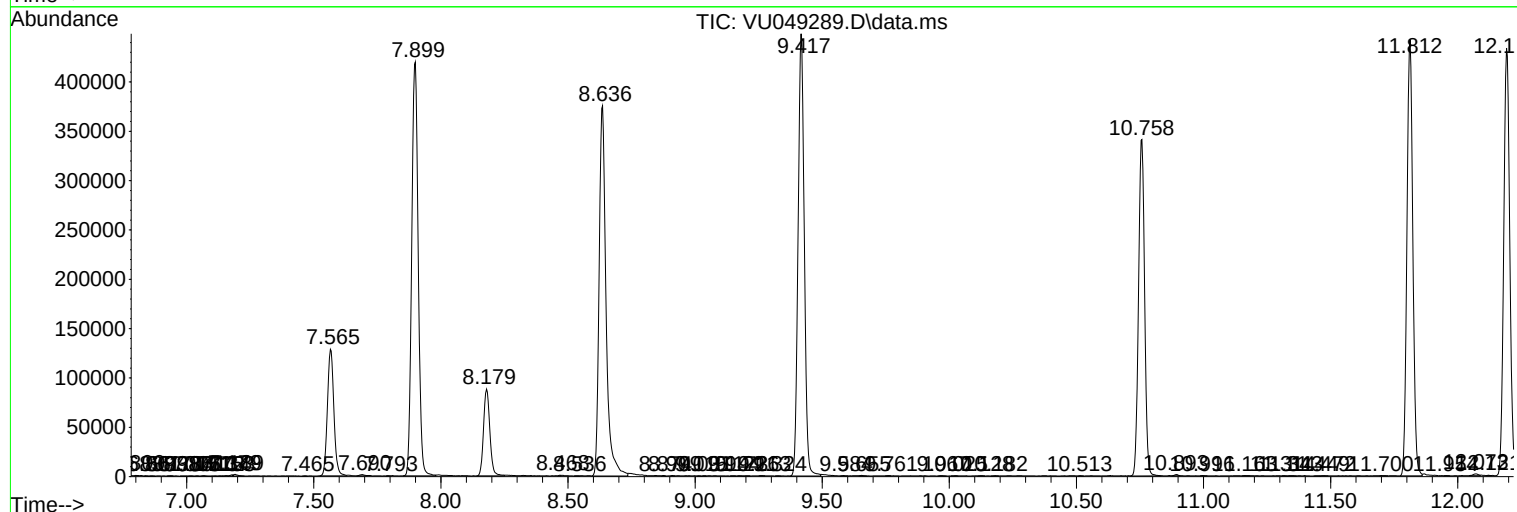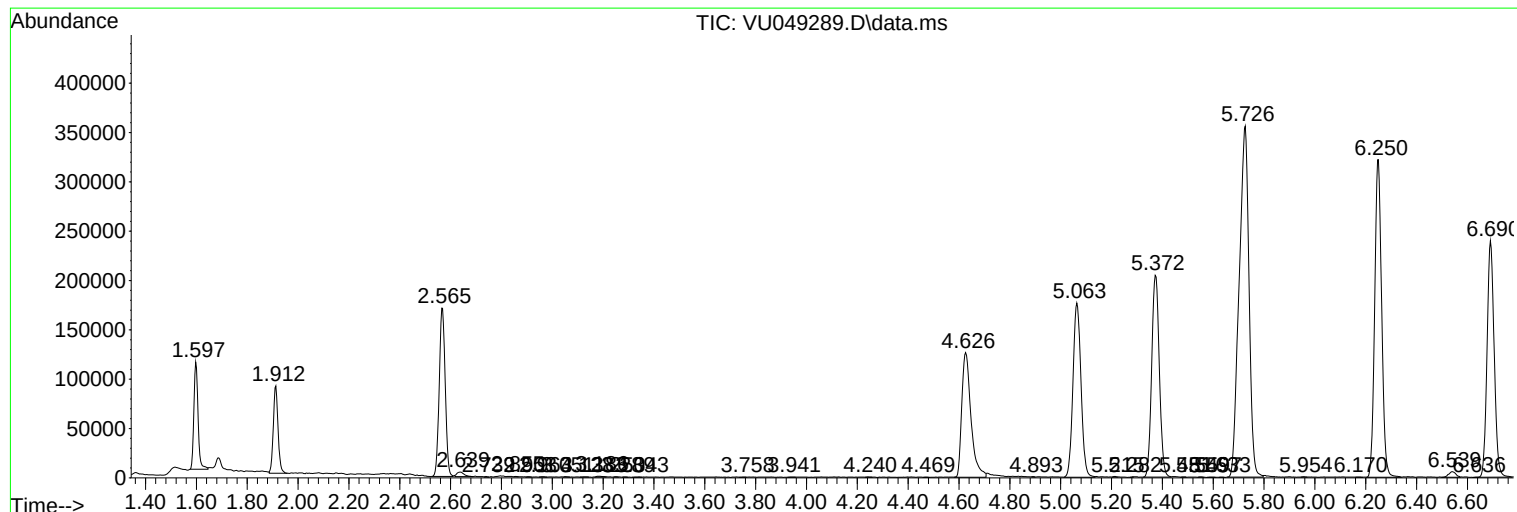

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
Data File : VU049289.D
Acq On : 18 Jun 2022 18:21
Operator : SY/MD
Sample : N3313-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
Data File : VU049289.D
Acq On : 18 Jun 2022 18:21
Operator : SY/MD
Sample : N3313-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------