

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
 Data File : VU049291.D
 Acq On : 18 Jun 2022 19:08
 Operator : SY/MD
 Sample : N3395-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0154

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049291.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	16	rVB3	4717	4178	0.42%	0.048%
2	1.485	36	45	55	rBV2	13444	30510	3.10%	0.353%
3	1.597	73	80	98	rVB	121910	138223	14.03%	1.601%
4	1.912	170	178	193	rVB	95788	124453	12.63%	1.442%
5	2.568	369	382	395	rBV	185138	305485	31.00%	3.539%
6	2.861	467	473	476	rBV3	325	425	0.04%	0.005%
7	3.176	568	571	572	rBV2	434	293	0.03%	0.003%
8	3.408	640	643	645	rBV	353	233	0.02%	0.003%
9	3.478	660	665	672	rBV3	322	456	0.05%	0.005%
10	3.639	710	715	722	rVV3	282	373	0.04%	0.004%
11	3.752	745	750	756	rVB3	292	286	0.03%	0.003%
12	3.848	776	780	784	rBV2	296	328	0.03%	0.004%
13	4.009	827	830	834	rVB3	257	211	0.02%	0.002%
14	4.038	834	839	842	rBV2	366	320	0.03%	0.004%
15	4.063	842	847	851	rVV3	220	240	0.02%	0.003%
16	4.131	865	868	872	rVB2	340	281	0.03%	0.003%
17	4.260	903	908	914	rBV3	399	612	0.06%	0.007%
18	4.398	946	951	953	rBV2	291	256	0.03%	0.003%
19	4.427	957	960	968	rBV2	338	354	0.04%	0.004%
20	4.488	975	979	986	rBV3	383	548	0.06%	0.006%
21	4.539	992	995	997	rBV2	262	195	0.02%	0.002%
22	4.620	1007	1020	1049	rBV	120239	291987	29.63%	3.383%
23	5.063	1141	1158	1177	rBV	180211	398496	40.44%	4.617%
24	5.182	1193	1195	1199	rVB3	615	450	0.05%	0.005%
25	5.208	1199	1203	1208	rBV5	619	689	0.07%	0.008%
26	5.372	1238	1254	1274	rBV	236486	483022	49.02%	5.596%
27	5.726	1342	1364	1387	rBV2	363557	985366	100.00%	11.417%
28	5.903	1416	1419	1421	rBV	354	229	0.02%	0.003%
29	6.182	1502	1506	1508	rVB	221	192	0.02%	0.002%
30	6.247	1508	1526	1544	rBV	353563	673995	68.40%	7.809%
31	6.398	1570	1573	1578	rBV4	274	241	0.02%	0.003%
32	6.530	1603	1614	1615	rBV6	2225	2508	0.25%	0.029%
33	6.571	1625	1627	1632	rVB2	401	278	0.03%	0.003%
34	6.594	1632	1634	1638	rVB3	432	277	0.03%	0.003%
35	6.690	1649	1664	1684	rBV	242525	471864	47.89%	5.467%
36	6.809	1699	1701	1710	rVB5	881	927	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
 Data File : VU049291.D
 Acq On : 18 Jun 2022 19:08
 Operator : SY/MD
 Sample : N3395-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0154

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.906	1729	1731	1737	rVB3	471	451	0.05%	0.005%
38	6.964	1746	1749	1752	rBV2	270	186	0.02%	0.002%
39	7.005	1757	1762	1764	rVB3	261	243	0.02%	0.003%
40	7.112	1791	1795	1797	rBV2	370	262	0.03%	0.003%
41	7.182	1808	1817	1825	rBV4	1436	2479	0.25%	0.029%
42	7.317	1853	1859	1863	rBV	272	289	0.03%	0.003%
43	7.504	1914	1917	1921	rVB2	427	343	0.03%	0.004%
44	7.565	1921	1936	1959	rBV	130716	230864	23.43%	2.675%
45	7.677	1967	1971	1973	rBV3	787	593	0.06%	0.007%
46	7.767	1996	1999	2002	rBV3	313	280	0.03%	0.003%
47	7.832	2014	2019	2024	rVB3	237	245	0.02%	0.003%
48	7.899	2026	2040	2060	rBV	451516	783640	79.53%	9.079%
49	8.047	2083	2086	2089	rBV2	551	366	0.04%	0.004%
50	8.179	2115	2127	2150	rBV	89181	151013	15.33%	1.750%
51	8.285	2156	2160	2163	rBV4	404	278	0.03%	0.003%
52	8.349	2178	2180	2184	rVB2	250	198	0.02%	0.002%
53	8.375	2184	2188	2194	rVB3	608	656	0.07%	0.008%
54	8.417	2194	2201	2208	rBV	552	886	0.09%	0.010%
55	8.468	2213	2217	2230	rVB3	757	1191	0.12%	0.014%
56	8.632	2253	2268	2296	rBV	341033	653293	66.30%	7.569%
57	8.874	2337	2343	2346	rBV3	215	246	0.02%	0.003%
58	8.893	2346	2349	2352	rVB3	385	257	0.03%	0.003%
59	8.912	2352	2355	2360	rBV3	307	276	0.03%	0.003%
60	9.083	2404	2408	2411	rBV2	194	189	0.02%	0.002%
61	9.134	2421	2424	2430	rVB2	212	227	0.02%	0.003%
62	9.253	2457	2461	2465	rBV2	367	323	0.03%	0.004%
63	9.417	2498	2512	2550	rVB	479812	814941	82.70%	9.442%
64	9.648	2580	2584	2586	rBV2	486	404	0.04%	0.005%
65	9.661	2586	2588	2592	rVB2	562	336	0.03%	0.004%
66	9.738	2609	2612	2614	rBV2	323	223	0.02%	0.003%
67	9.919	2663	2668	2671	rBV3	236	218	0.02%	0.003%
68	10.012	2693	2697	2701	rBV2	278	269	0.03%	0.003%
69	10.214	2755	2760	2766	rBV3	272	272	0.03%	0.003%
70	10.285	2775	2782	2784	rBV	255	267	0.03%	0.003%
71	10.317	2789	2792	2799	rVB3	208	203	0.02%	0.002%
72	10.391	2811	2815	2819	rVB2	341	317	0.03%	0.004%
73	10.417	2820	2823	2826	rBV2	297	186	0.02%	0.002%
74	10.465	2835	2838	2841	rBV	313	228	0.02%	0.003%
75	10.542	2857	2862	2866	rBV3	296	322	0.03%	0.004%
76	10.600	2878	2880	2883	rVB2	314	211	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
 Data File : VU049291.D
 Acq On : 18 Jun 2022 19:08
 Operator : SY/MD
 Sample : N3395-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0154

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	10.668	2894	2901	2905	rBV2	243	400	0.04%	0.005%
78	10.755	2916	2928	2954	rBV	336807	551759	56.00%	6.393%
79	10.877	2963	2966	2968	rBV	439	321	0.03%	0.004%
80	10.893	2969	2971	2973	rVV2	480	270	0.03%	0.003%
81	10.983	2994	2999	3002	rBV	256	234	0.02%	0.003%
82	11.346	3107	3112	3121	rBV3	224	373	0.04%	0.004%
83	11.722	3223	3229	3231	rBV2	361	373	0.04%	0.004%
84	11.812	3244	3257	3273	rBV	491074	772156	78.36%	8.946%
85	12.082	3339	3341	3343	rBV3	315	188	0.02%	0.002%
86	12.192	3362	3375	3401	rBV	448223	734665	74.56%	8.512%
87	12.381	3431	3434	3438	rBV2	202	228	0.02%	0.003%
88	12.761	3549	3552	3553	rBV2	387	186	0.02%	0.002%
89	13.092	3651	3655	3658	rBV2	293	267	0.03%	0.003%
90	13.780	3866	3869	3873	rBV2	303	204	0.02%	0.002%
91	14.336	4039	4042	4044	rBV2	497	318	0.03%	0.004%
92	14.629	4131	4133	4137	rBV	271	197	0.02%	0.002%
93	14.790	4181	4183	4186	rBV2	307	194	0.02%	0.002%
94	15.240	4321	4323	4328	rVB3	481	295	0.03%	0.003%
95	15.266	4328	4331	4333	rBV2	326	195	0.02%	0.002%
96	15.375	4362	4365	4369	rVB2	574	371	0.04%	0.004%
97	15.397	4369	4372	4374	rBV2	472	226	0.02%	0.003%
98	15.452	4387	4389	4392	rBV	403	269	0.03%	0.003%
99	16.172	4611	4613	4616	rBV3	639	385	0.04%	0.004%
100	16.529	4721	4724	4726	rBV2	794	542	0.06%	0.006%


Sum of corrected areas: 8631068

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
Data File : VU049291.D
Acq On : 18 Jun 2022 19:08
Operator : SY/MD
Sample : N3395-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0154

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

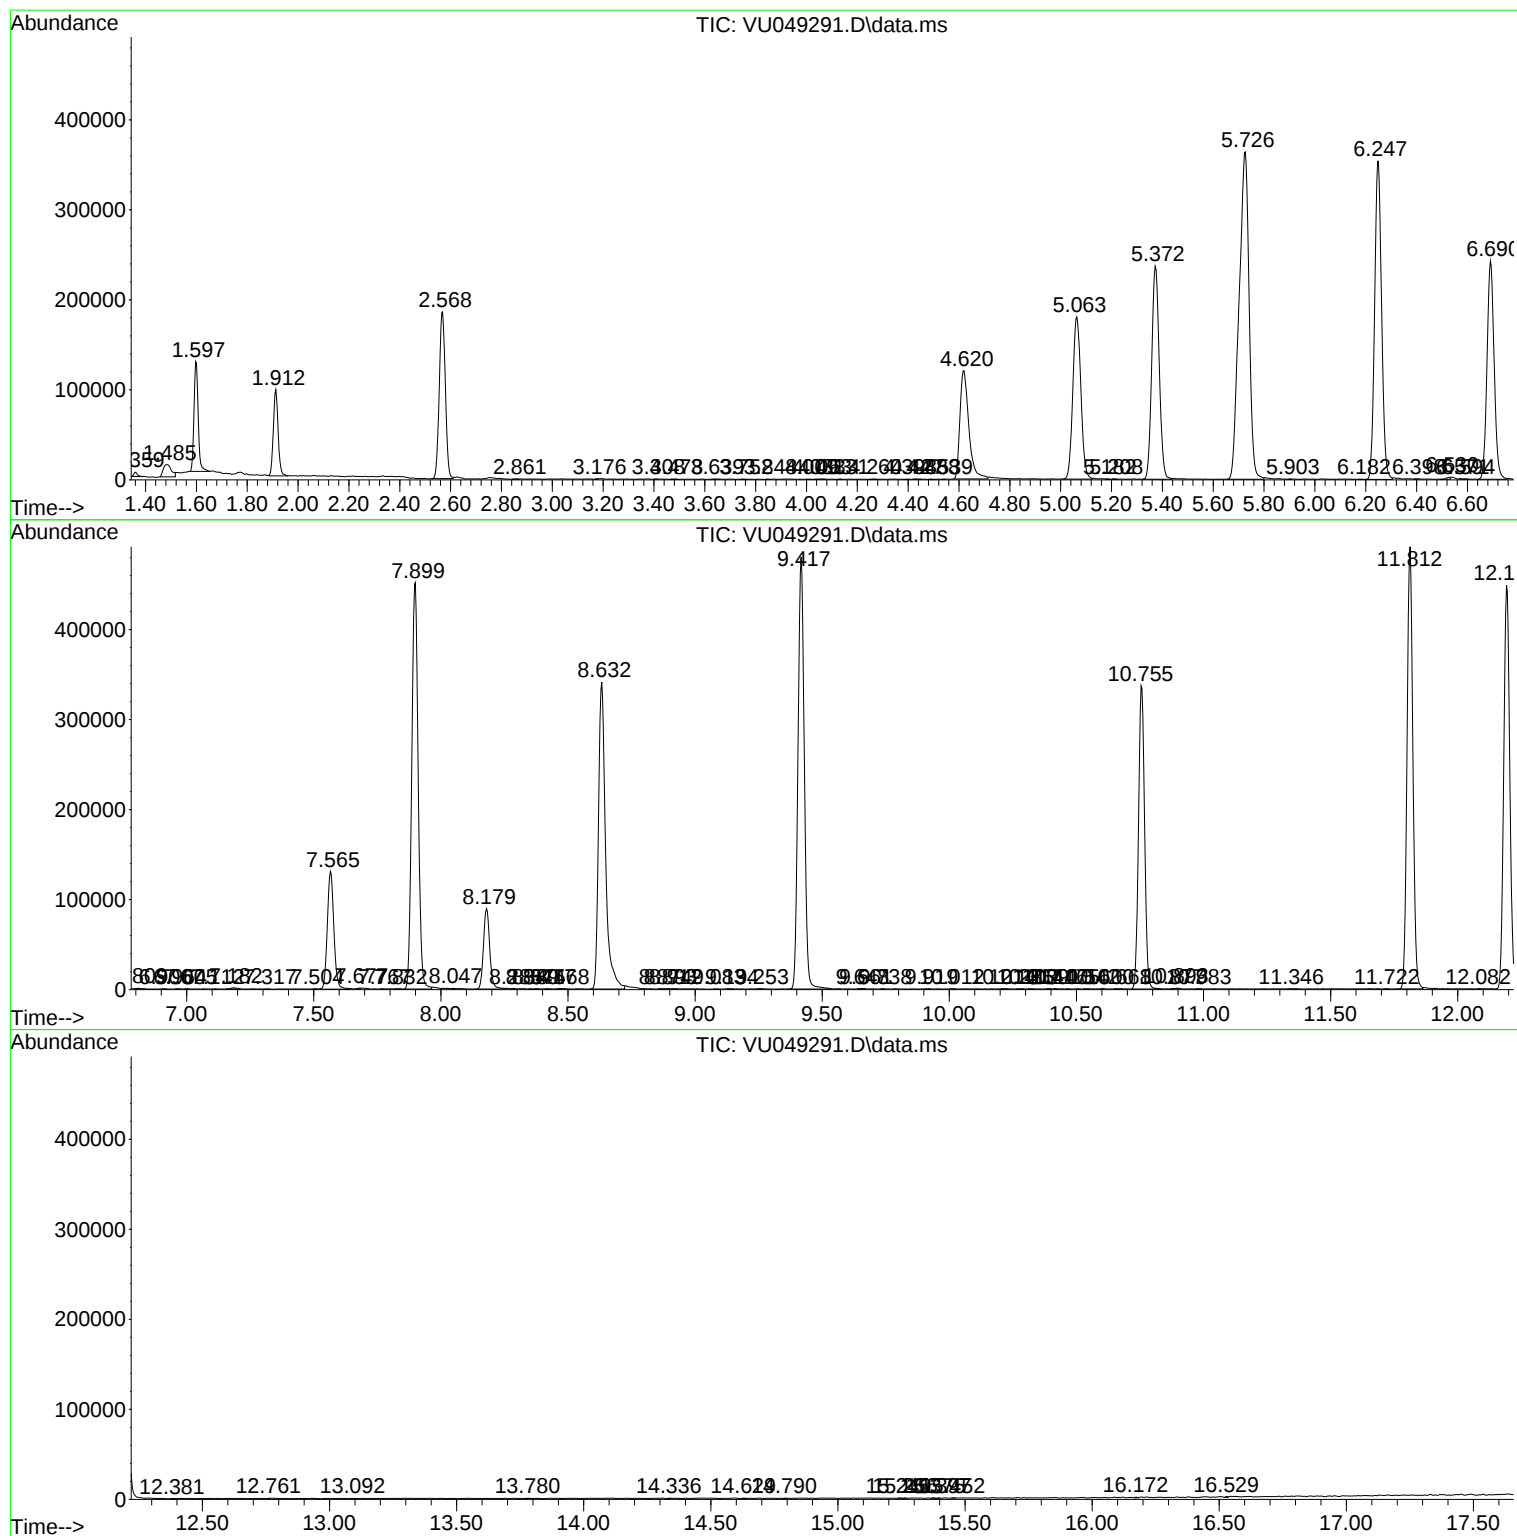

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
Data File : VU049291.D
Acq On : 18 Jun 2022 19:08
Operator : SY/MD
Sample : N3395-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0154

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061822\
Data File : VU049291.D
Acq On : 18 Jun 2022 19:08
Operator : SY/MD
Sample : N3395-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0154

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------